

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042860.D
 Acq On : 18 Nov 2023 00:56
 Operator : MA/JU
 Sample : 05226-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	37	rVB4	6795	8712	0.89%	0.126%
2	3.628	106	109	120	rBV2	15674	32863	3.35%	0.475%
3	4.610	275	276	281	rBV4	1649	2517	0.26%	0.036%
4	4.852	315	317	318	rBV2	1316	991	0.10%	0.014%
5	5.216	377	379	382	rBV4	1085	1325	0.14%	0.019%
6	5.463	420	421	423	rBV2	1239	1029	0.11%	0.015%
7	5.993	509	511	515	rVB3	1134	1073	0.11%	0.016%
8	6.193	544	545	548	rBV3	1037	1032	0.11%	0.015%
9	6.834	652	654	656	rVB3	1248	982	0.10%	0.014%
10	6.998	677	682	693	rBV4	13032	35240	3.60%	0.509%
11	7.169	705	711	723	rBV	88805	167282	17.07%	2.417%
12	7.340	734	740	753	rBV	86780	169535	17.30%	2.450%
13	7.610	784	786	788	rVB2	1580	986	0.10%	0.014%
14	7.687	796	799	801	rBV4	1352	1327	0.14%	0.019%
15	7.822	816	822	833	rBV	72772	138740	14.16%	2.005%
16	8.545	940	945	962	rBV	47087	106394	10.86%	1.537%
17	9.022	1020	1026	1041	rBV	107903	220474	22.50%	3.186%
18	9.122	1041	1043	1045	rVB2	1272	1097	0.11%	0.016%
19	9.269	1064	1068	1069	rVB3	1122	1404	0.14%	0.020%
20	9.522	1108	1111	1114	rBV4	762	1063	0.11%	0.015%
21	9.734	1140	1147	1163	rBV	87976	181393	18.51%	2.621%
22	9.834	1163	1164	1170	rVV4	2906	4124	0.42%	0.060%
23	10.263	1231	1237	1255	rBV2	87024	202502	20.67%	2.926%
24	10.451	1268	1269	1275	rVB4	1486	2191	0.22%	0.032%
25	10.492	1275	1276	1279	rBV3	1292	987	0.10%	0.014%
26	10.634	1293	1300	1309	rBV	103040	180608	18.43%	2.610%
27	10.816	1325	1331	1345	rBV2	58016	154882	15.81%	2.238%
28	11.134	1384	1385	1388	rBV2	1371	1145	0.12%	0.017%
29	11.175	1388	1392	1394	rVV3	808	1180	0.12%	0.017%
30	11.592	1458	1463	1467	rBV4	854	1703	0.17%	0.025%
31	12.728	1653	1656	1657	rBV3	825	1025	0.10%	0.015%
32	12.792	1660	1667	1672	rVV4	2053	3568	0.36%	0.052%
33	13.057	1706	1712	1717	rVB3	2670	4156	0.42%	0.060%
34	13.316	1753	1756	1764	rVB6	1597	3107	0.32%	0.045%
35	13.898	1849	1855	1867	rBV	279536	403235	41.16%	5.827%
36	14.051	1878	1881	1885	rVB5	751	1283	0.13%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042860.D
 Acq On : 18 Nov 2023 00:56
 Operator : MA/JU
 Sample : 05226-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.175	1896	1902	1916	rBV	294793	433335	44.23%	6.262%
38	14.474	1948	1953	1962	rVV	147218	221626	22.62%	3.203%
39	14.863	2018	2019	2023	rBV4	902	1012	0.10%	0.015%
40	15.251	2084	2085	2088	rBV2	953	1094	0.11%	0.016%
41	15.469	2115	2122	2137	rBV	368426	562296	57.39%	8.126%
42	15.621	2143	2148	2160	rBV2	85760	156981	16.02%	2.268%
43	15.880	2189	2192	2195	rBV3	689	1081	0.11%	0.016%
44	16.145	2234	2237	2241	rVB3	695	1056	0.11%	0.015%
45	16.639	2318	2321	2323	rVB2	985	1028	0.10%	0.015%
46	17.227	2415	2421	2432	rBV	175716	256716	26.20%	3.710%
47	17.327	2432	2438	2456	rVV	452226	678184	69.22%	9.800%
48	17.474	2461	2463	2466	rVB2	1451	1586	0.16%	0.023%
49	18.086	2564	2567	2578	rVV9	4274	10498	1.07%	0.152%
50	18.445	2624	2628	2630	rVB4	823	1016	0.10%	0.015%
51	18.480	2630	2634	2637	rBV4	1400	1757	0.18%	0.025%
52	18.639	2659	2661	2664	rBV2	1220	1466	0.15%	0.021%
53	18.768	2679	2683	2685	rBV5	954	1279	0.13%	0.018%
54	19.051	2728	2731	2732	rBV3	1268	1101	0.11%	0.016%
55	19.133	2743	2745	2749	rVB6	1119	1212	0.12%	0.018%
56	19.192	2751	2755	2759	rVV5	4322	5782	0.59%	0.084%
57	19.268	2763	2768	2773	rBV4	2990	5104	0.52%	0.074%
58	19.374	2783	2786	2789	rBV6	2256	3126	0.32%	0.045%
59	19.627	2823	2829	2843	rBV	637176	886721	90.50%	12.814%
60	19.798	2855	2858	2862	rBV5	1174	2308	0.24%	0.033%
61	19.921	2877	2879	2881	rBV3	2615	2817	0.29%	0.041%
62	19.992	2889	2891	2893	rBV2	1696	1118	0.11%	0.016%
63	20.492	2974	2976	2977	rBV2	2100	1220	0.12%	0.018%
64	21.415	3128	3133	3146	rBV	192638	299738	30.59%	4.331%
65	23.615	3500	3507	3524	rBV	473612	979764	100.00%	14.158%
66	23.774	3528	3534	3549	rVB	156900	356867	36.42%	5.157%




Sum of corrected areas: 6920044

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042860.D
Acq On : 18 Nov 2023 00:56
Operator : MA/JU
Sample : 05226-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

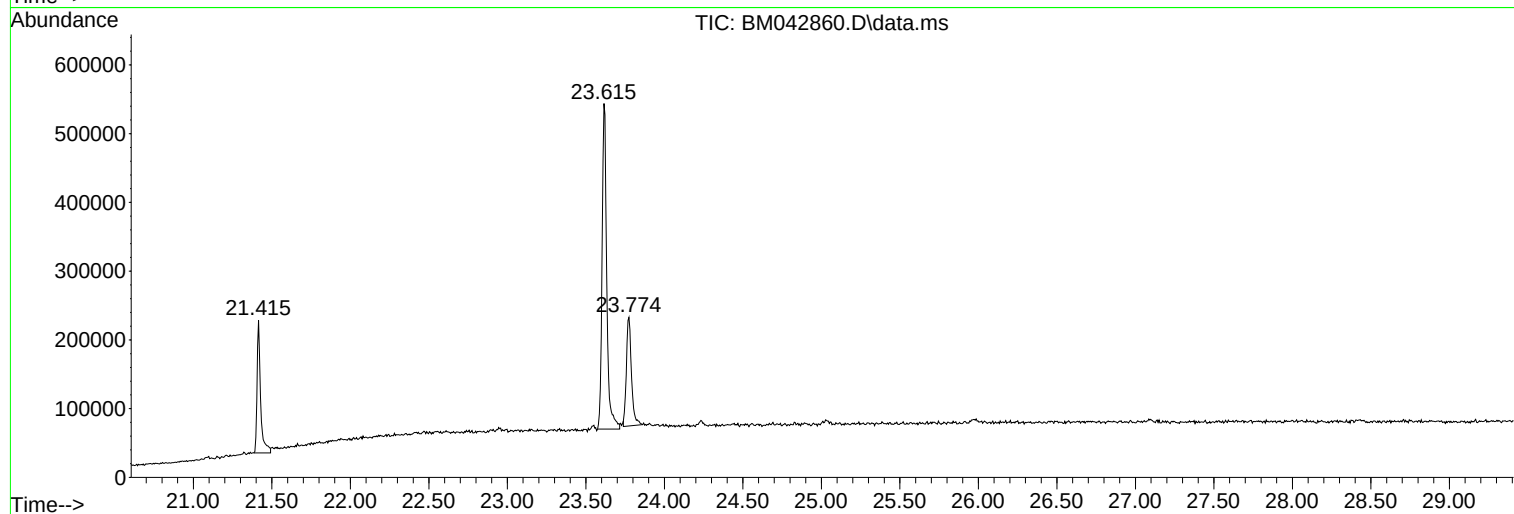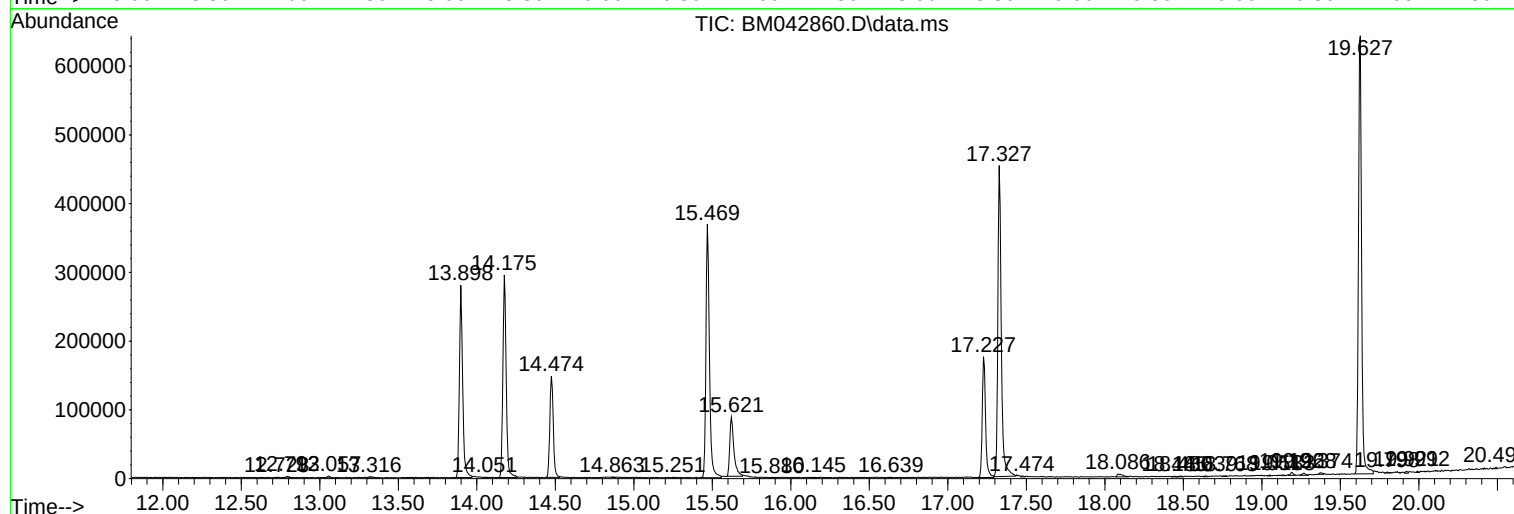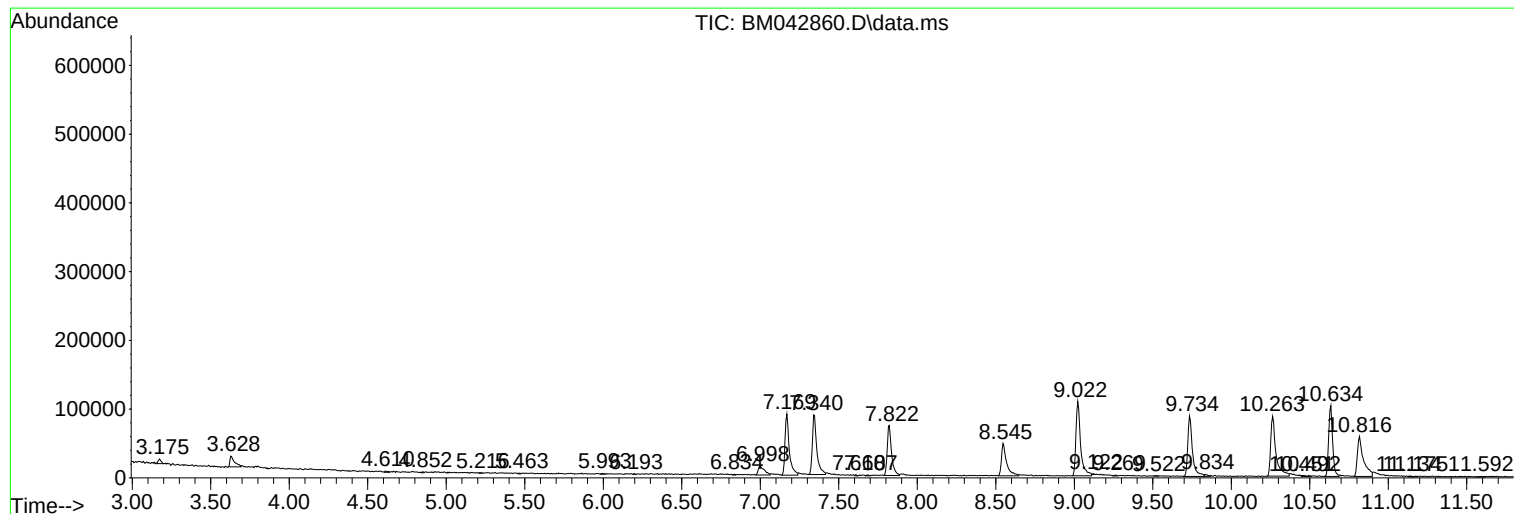

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042860.D
Acq On : 18 Nov 2023 00:56
Operator : MA/JU
Sample : 05226-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042860.D
Acq On : 18 Nov 2023 00:56
Operator : MA/JU
Sample : 05226-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc