

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042864.D
 Acq On : 18 Nov 2023 03:23
 Operator : MA/JU
 Sample : 05226-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	40	rVB5	8191	12098	1.26%	0.160%
2	3.622	105	108	120	rBV	34874	71408	7.43%	0.942%
3	4.569	268	269	271	rBV	1647	1095	0.11%	0.014%
4	5.357	402	403	407	rBV4	1032	1107	0.12%	0.015%
5	5.634	448	450	452	rBV3	1390	1391	0.14%	0.018%
6	5.834	483	484	486	rBV2	1778	1234	0.13%	0.016%
7	5.875	490	491	494	rBV3	1470	1303	0.14%	0.017%
8	5.934	499	501	504	rVV3	1344	1495	0.16%	0.020%
9	5.993	507	511	513	rBV4	1097	1196	0.12%	0.016%
10	6.075	521	525	526	rBV4	903	1245	0.13%	0.016%
11	6.128	533	534	537	rBV3	1093	1462	0.15%	0.019%
12	6.587	609	612	615	rBV4	1157	1100	0.11%	0.015%
13	6.993	677	681	692	rBV2	17235	43187	4.49%	0.569%
14	7.169	704	711	728	rBV	106045	196158	20.41%	2.587%
15	7.340	735	740	751	rBV	107055	197594	20.56%	2.605%
16	7.816	816	821	835	rBV	86037	162271	16.88%	2.140%
17	7.998	849	852	854	rBV2	1181	1049	0.11%	0.014%
18	8.545	940	945	960	rBV2	58666	130741	13.60%	1.724%
19	9.022	1019	1026	1041	rBV	129896	255730	26.60%	3.372%
20	9.298	1072	1073	1077	rVB4	1203	1522	0.16%	0.020%
21	9.334	1077	1079	1082	rBV4	1307	1369	0.14%	0.018%
22	9.734	1141	1147	1159	rBV2	103201	200944	20.90%	2.650%
23	10.263	1230	1237	1254	rBV	109463	245863	25.58%	3.242%
24	10.445	1267	1268	1272	rVB3	1727	1426	0.15%	0.019%
25	10.628	1293	1299	1313	rBV	118308	215243	22.39%	2.838%
26	10.733	1315	1317	1321	rVB4	842	1119	0.12%	0.015%
27	10.810	1324	1330	1350	rBV	78395	208414	21.68%	2.748%
28	10.980	1358	1359	1365	rVB5	1247	1951	0.20%	0.026%
29	11.692	1478	1480	1485	rVB5	1268	1639	0.17%	0.022%
30	11.939	1518	1522	1526	rVV4	600	1011	0.11%	0.013%
31	12.380	1593	1597	1601	rVB5	566	979	0.10%	0.013%
32	12.892	1680	1684	1687	rBV3	1024	1363	0.14%	0.018%
33	13.322	1752	1757	1765	rVV4	2476	4340	0.45%	0.057%
34	13.898	1849	1855	1867	rVV	309566	439294	45.70%	5.792%
35	13.992	1870	1871	1877	rVB3	1195	1552	0.16%	0.020%
36	14.174	1896	1902	1918	rBV	338242	480687	50.01%	6.338%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042864.D
 Acq On : 18 Nov 2023 03:23
 Operator : MA/JU
 Sample : 05226-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.474	1948	1953	1963	rVV	177786	256562	26.69%	3.383%
38	14.568	1966	1969	1972	rVB4	950	1230	0.13%	0.016%
39	14.798	2006	2008	2018	rVV4	1573	3966	0.41%	0.052%
40	15.068	2051	2054	2057	rBV3	800	1319	0.14%	0.017%
41	15.215	2073	2079	2082	rVB3	1388	1780	0.19%	0.023%
42	15.257	2082	2086	2090	rBV4	2519	3862	0.40%	0.051%
43	15.468	2116	2122	2134	rBV	415354	597759	62.19%	7.882%
44	15.621	2142	2148	2161	rBV	97477	180767	18.81%	2.384%
45	15.704	2161	2162	2169	rVV4	3170	4521	0.47%	0.060%
46	16.039	2214	2219	2220	rVB2	959	1095	0.11%	0.014%
47	17.227	2416	2421	2432	rBV	203673	295382	30.73%	3.895%
48	17.327	2432	2438	2456	rVV	469448	691331	71.92%	9.116%
49	17.639	2489	2491	2495	rBV5	998	1066	0.11%	0.014%
50	17.727	2501	2506	2507	rBV2	724	1159	0.12%	0.015%
51	17.757	2510	2511	2514	rVB3	1191	1033	0.11%	0.014%
52	17.857	2524	2528	2534	rVB4	2200	3012	0.31%	0.040%
53	18.080	2563	2566	2573	rVV3	9288	16515	1.72%	0.218%
54	18.133	2573	2575	2578	rVV3	1759	1931	0.20%	0.025%
55	18.345	2607	2611	2612	rBV3	822	1101	0.11%	0.015%
56	18.651	2660	2663	2666	rVB3	1242	1231	0.13%	0.016%
57	18.686	2666	2669	2671	rBV3	853	1169	0.12%	0.015%
58	18.827	2691	2693	2694	rBV2	1363	1187	0.12%	0.016%
59	18.903	2700	2706	2709	rVB5	1574	1827	0.19%	0.024%
60	18.939	2709	2712	2714	rBV4	1205	1241	0.13%	0.016%
61	19.003	2722	2723	2725	rBV2	1466	1413	0.15%	0.019%
62	19.186	2751	2754	2757	rBV4	4514	5464	0.57%	0.072%
63	19.256	2763	2766	2770	rBV4	3747	5309	0.55%	0.070%
64	19.362	2782	2784	2791	rVB7	3483	5320	0.55%	0.070%
65	19.551	2814	2816	2818	rBV3	1692	1456	0.15%	0.019%
66	19.621	2823	2828	2842	rBV	673376	907590	94.42%	11.967%
67	19.821	2860	2862	2864	rBV3	1705	1279	0.13%	0.017%
68	20.015	2893	2895	2896	rBV2	1578	1234	0.13%	0.016%
69	20.139	2914	2916	2918	rBV3	2082	1067	0.11%	0.014%
70	21.415	3128	3133	3141	rBV	214756	331722	34.51%	4.374%
71	23.615	3500	3507	3522	rBV2	476027	961251	100.00%	12.675%
72	23.768	3527	3533	3547	rVB	181891	397111	41.31%	5.236%




Sum of corrected areas: 7583842

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042864.D
Acq On : 18 Nov 2023 03:23
Operator : MA/JU
Sample : 05226-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

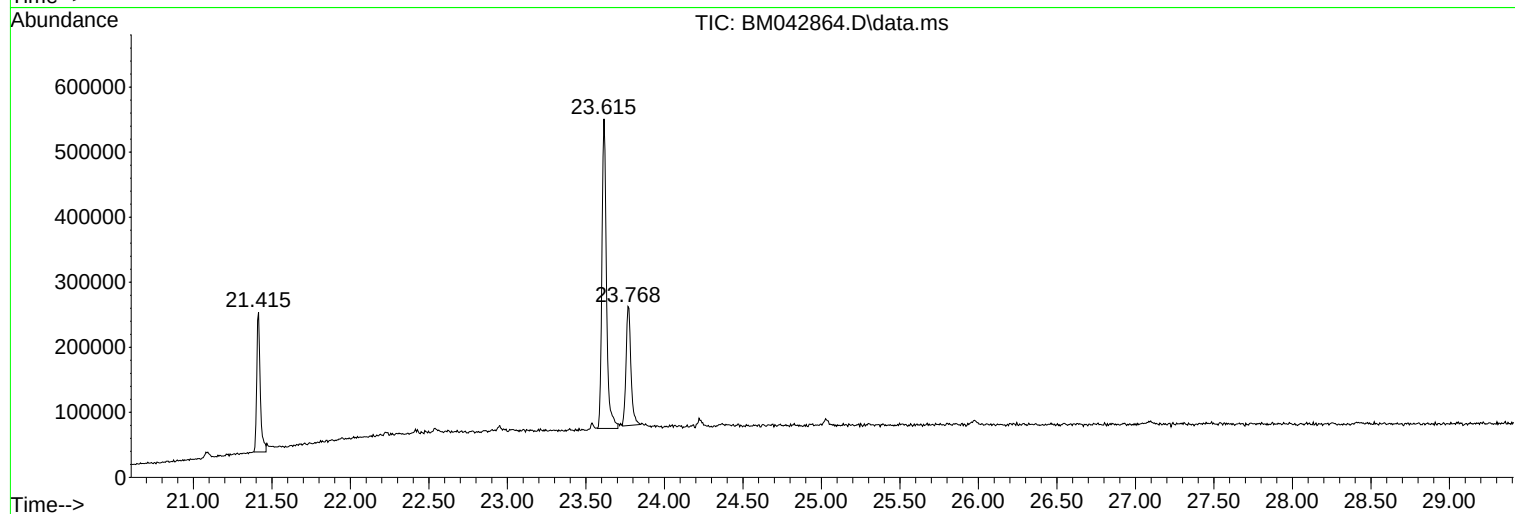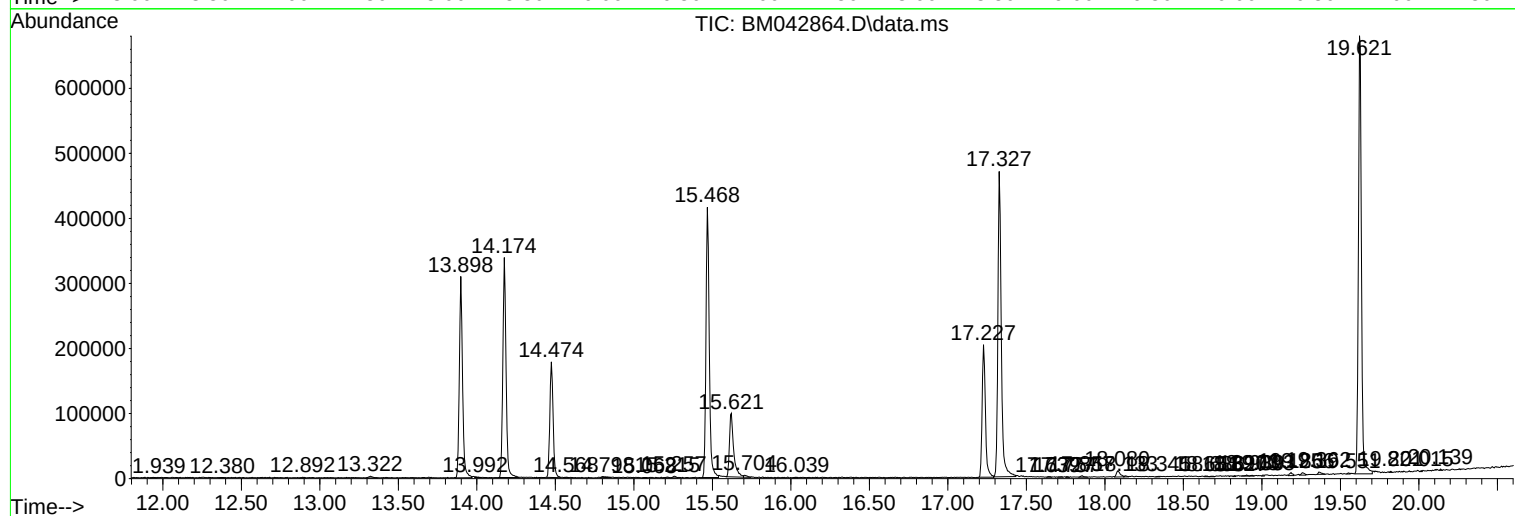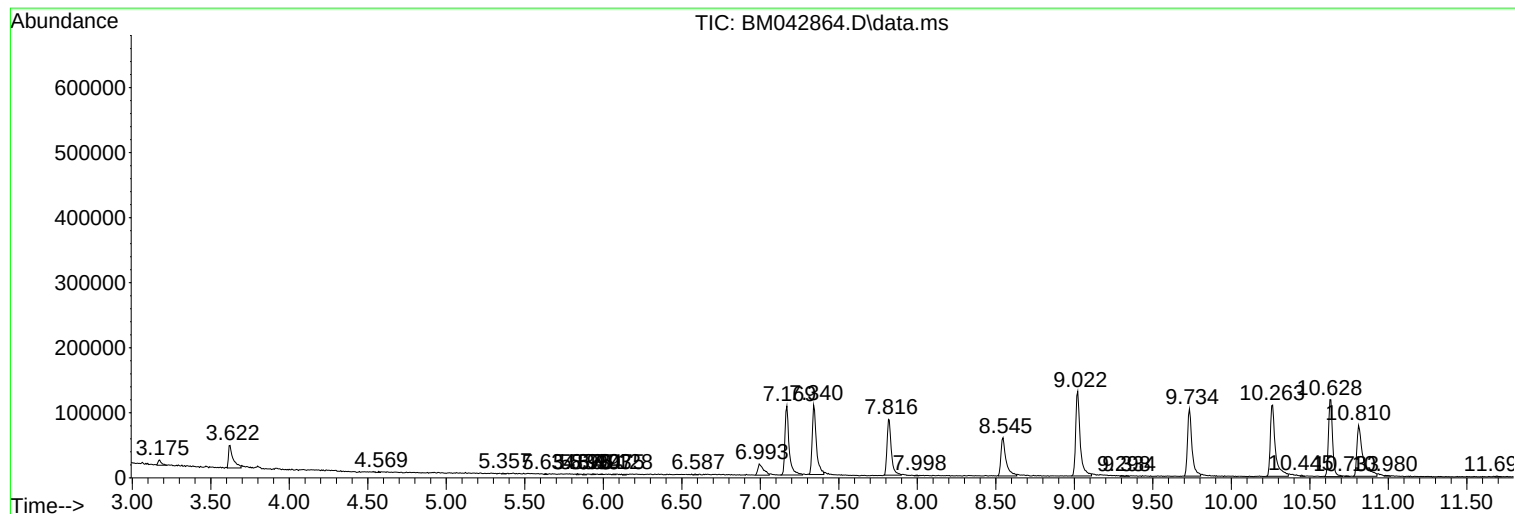

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042864.D
Acq On : 18 Nov 2023 03:23
Operator : MA/JU
Sample : 05226-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042864.D
Acq On : 18 Nov 2023 03:23
Operator : MA/JU
Sample : 05226-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------