

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042865.D
 Acq On : 18 Nov 2023 03:59
 Operator : MA/JU
 Sample : 05226-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	37	rVB2	7076	8967	0.93%	0.117%
2	3.622	105	108	117	rBV2	31710	60298	6.24%	0.786%
3	3.916	156	158	162	rVB4	3688	4872	0.50%	0.064%
4	5.222	378	380	383	rBV3	1140	1315	0.14%	0.017%
5	5.698	459	461	464	rBV3	922	983	0.10%	0.013%
6	6.169	538	541	544	rBV3	1445	1506	0.16%	0.020%
7	6.328	565	568	573	rBV4	1655	2552	0.26%	0.033%
8	6.487	592	595	597	rVB5	1363	1625	0.17%	0.021%
9	6.934	670	671	674	rBV3	1046	1191	0.12%	0.016%
10	6.998	677	682	696	rVV2	13612	37954	3.93%	0.495%
11	7.169	705	711	725	rBV	108338	200670	20.77%	2.616%
12	7.345	735	741	753	rBV	99798	190636	19.73%	2.485%
13	7.822	816	822	833	rBV	88856	166313	17.21%	2.168%
14	7.992	848	851	854	rVB3	1061	1342	0.14%	0.017%
15	8.022	854	856	859	rBV3	829	1089	0.11%	0.014%
16	8.545	939	945	965	rBV	54924	123704	12.80%	1.613%
17	8.686	967	969	973	rVB4	909	1131	0.12%	0.015%
18	9.022	1020	1026	1039	rBV	134105	266935	27.63%	3.480%
19	9.204	1055	1057	1060	rVB3	2048	1614	0.17%	0.021%
20	9.322	1074	1077	1080	rBV5	917	1202	0.12%	0.016%
21	9.363	1080	1084	1087	rVB5	965	1752	0.18%	0.023%
22	9.398	1087	1090	1094	rBV4	671	1029	0.11%	0.013%
23	9.733	1139	1147	1162	rBV2	107443	215238	22.28%	2.806%
24	10.257	1231	1236	1253	rBV2	106682	245848	25.45%	3.205%
25	10.633	1292	1300	1310	rBV	121346	217680	22.53%	2.838%
26	10.745	1313	1319	1320	rVB5	1299	1857	0.19%	0.024%
27	10.810	1324	1330	1348	rBV	85067	225576	23.35%	2.940%
28	11.110	1378	1381	1383	rVB3	1168	1268	0.13%	0.017%
29	11.557	1455	1457	1461	rVV3	950	1206	0.12%	0.016%
30	11.680	1475	1478	1480	rBV2	1395	1633	0.17%	0.021%
31	12.210	1564	1568	1572	rBV4	603	1031	0.11%	0.013%
32	12.339	1587	1590	1593	rVB4	870	1088	0.11%	0.014%
33	12.727	1651	1656	1657	rBV2	1455	1793	0.19%	0.023%
34	13.051	1709	1711	1716	rVB4	1406	1981	0.21%	0.026%
35	13.310	1750	1755	1764	rBV	46676	70429	7.29%	0.918%
36	13.704	1819	1822	1826	rVB4	1023	1528	0.16%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042865.D
 Acq On : 18 Nov 2023 03:59
 Operator : MA/JU
 Sample : 05226-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.898	1849	1855	1869	rBV	295951	436062	45.13%	5.684%
38	14.174	1896	1902	1917	rBV	344162	494447	51.18%	6.445%
39	14.474	1947	1953	1966	rVV	178417	266111	27.54%	3.469%
40	15.215	2076	2079	2082	rBV4	936	1079	0.11%	0.014%
41	15.468	2116	2122	2137	rBV	422187	612652	63.41%	7.986%
42	15.621	2143	2148	2161	rBV2	89419	168317	17.42%	2.194%
43	15.904	2194	2196	2199	rBV3	990	1215	0.13%	0.016%
44	16.051	2218	2221	2224	rVB3	1522	2035	0.21%	0.027%
45	16.521	2299	2301	2305	rVB3	880	1114	0.12%	0.015%
46	16.562	2305	2308	2311	rBV3	724	1008	0.10%	0.013%
47	17.127	2400	2404	2407	rVB5	787	1098	0.11%	0.014%
48	17.227	2416	2421	2432	rBV	203500	293969	30.43%	3.832%
49	17.327	2432	2438	2460	rVV	463625	705426	73.01%	9.195%
50	17.492	2464	2466	2467	rVV2	1555	1084	0.11%	0.014%
51	17.503	2467	2468	2472	rVB2	1352	1415	0.15%	0.018%
52	17.968	2544	2547	2550	rBV3	753	1119	0.12%	0.015%
53	18.056	2560	2562	2564	rBV2	943	1016	0.11%	0.013%
54	18.086	2564	2567	2574	rVV5	2514	5589	0.58%	0.073%
55	18.256	2594	2596	2599	rVB	1200	974	0.10%	0.013%
56	18.309	2601	2605	2608	rVV5	2307	3216	0.33%	0.042%
57	18.392	2616	2619	2622	rBV3	761	1117	0.12%	0.015%
58	18.450	2628	2629	2632	rBV2	1043	1101	0.11%	0.014%
59	18.745	2676	2679	2682	rVB3	759	1018	0.11%	0.013%
60	18.880	2701	2702	2704	rBV	1630	977	0.10%	0.013%
61	18.986	2718	2720	2722	rVB3	1508	1287	0.13%	0.017%
62	19.033	2724	2728	2730	rVV2	1269	1683	0.17%	0.022%
63	19.068	2730	2734	2735	rVV3	1106	1309	0.14%	0.017%
64	19.186	2751	2754	2760	rVB5	4202	5839	0.60%	0.076%
65	19.268	2764	2768	2769	rVV	3305	3813	0.39%	0.050%
66	19.292	2769	2772	2776	rVB	4756	5788	0.60%	0.075%
67	19.374	2781	2786	2789	rBV5	2023	3475	0.36%	0.045%
68	19.468	2801	2802	2804	rBV2	1892	1133	0.12%	0.015%
69	19.621	2823	2828	2843	rBV	660272	893762	92.50%	11.651%
70	19.939	2879	2882	2883	rBV3	1708	1553	0.16%	0.020%
71	20.721	3013	3015	3016	rBV2	3488	2954	0.31%	0.039%
72	21.415	3128	3133	3143	rBV	215770	340633	35.26%	4.440%
73	23.615	3500	3507	3520	rBV	481187	966187	100.00%	12.595%
74	23.774	3527	3534	3544	rVB	179173	372034	38.51%	4.850%

Sum of corrected areas: 7671445

Instrument :

BNA_M

ClientSampleId :




YCG47

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042865.D
Acq On : 18 Nov 2023 03:59
Operator : MA/JU
Sample : 05226-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

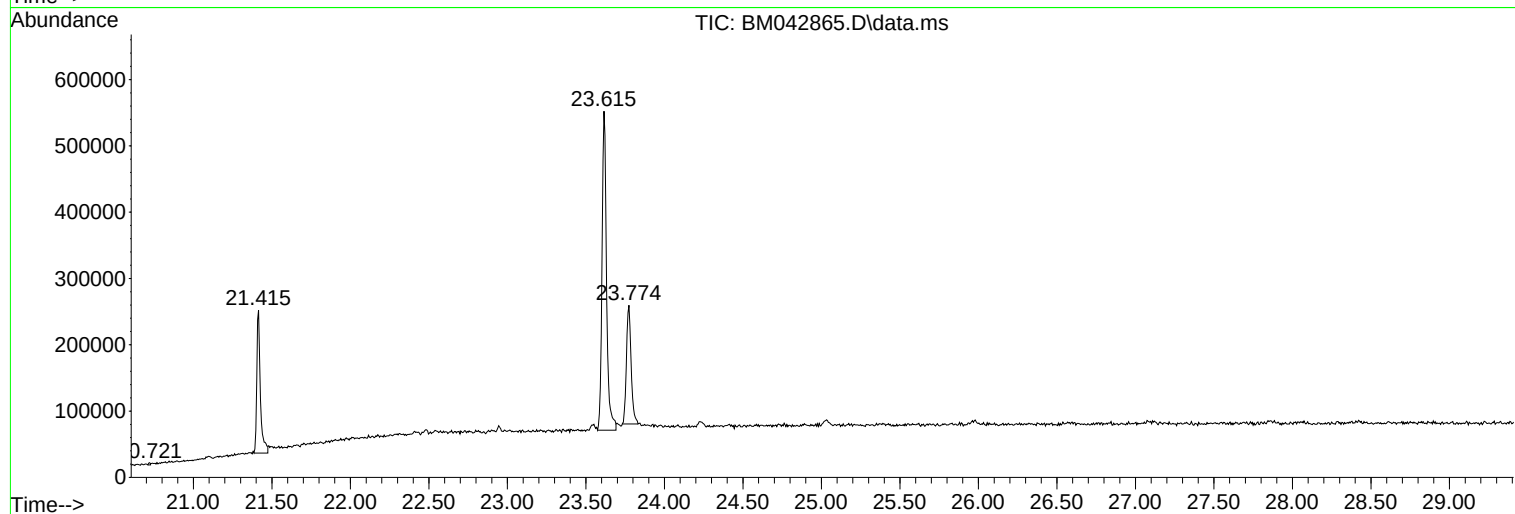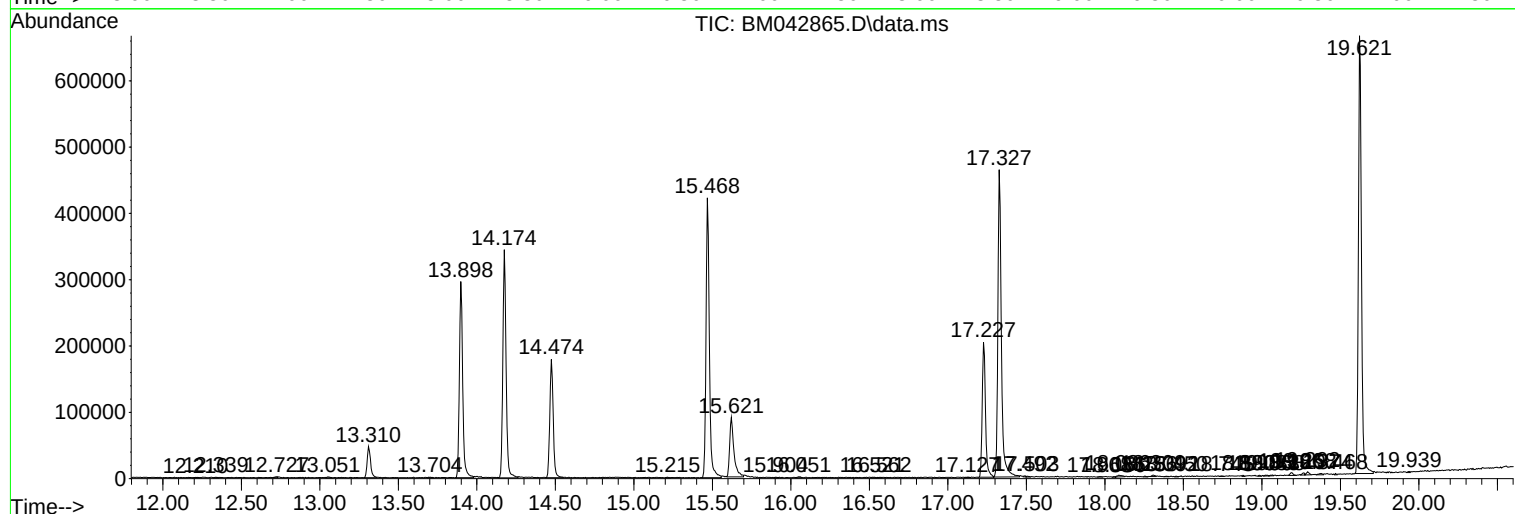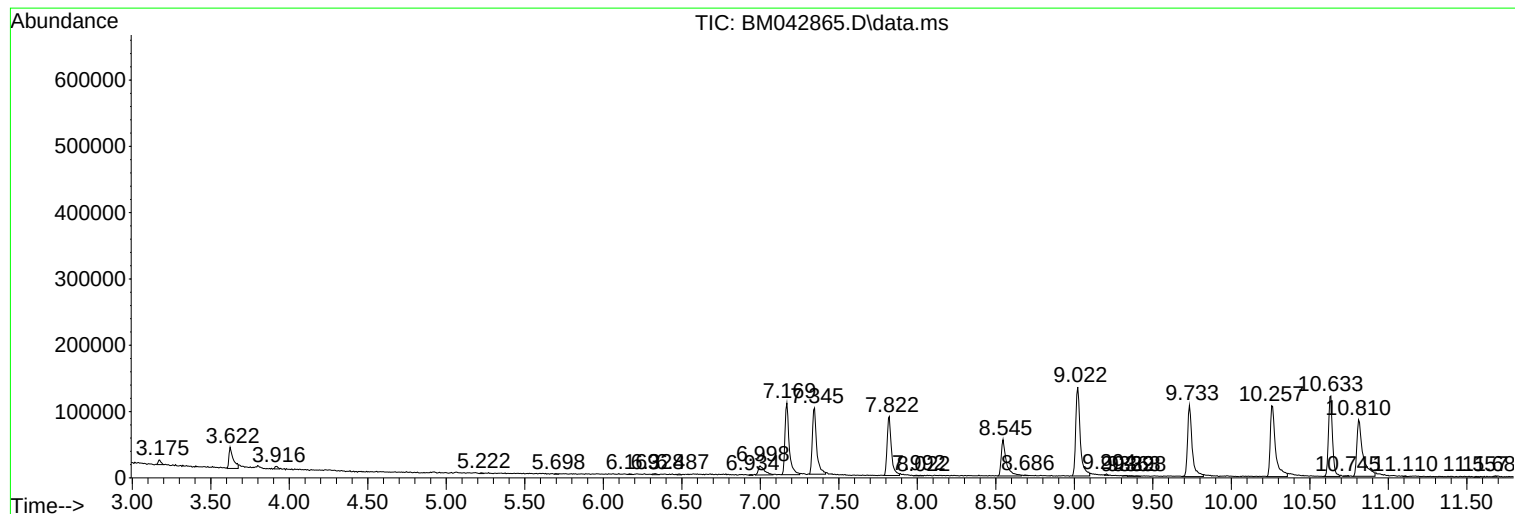

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042865.D
Acq On : 18 Nov 2023 03:59
Operator : MA/JU
Sample : 05226-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG47










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Phenol, 4-(1,1-dimethylprop... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.310	5.29 ng/ul	70429	Acenaphthene-d10	14.474

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, 4-(1,1-dimethylpropyl)-	164	C11H16O	000080-46-6	94
2			Phenol, 4-(1,1-dimethylpropyl)-	164	C11H16O	000080-46-6	91
3			Phenol, p-tert-butyl-	150	C10H14O	000098-54-4	72
4			Hexestrol	270	C18H22O2	000084-16-2	72
5			Hexestrol, O-trifluoroacetyl-	366	C20H21F3O3	1000365-31-7	64

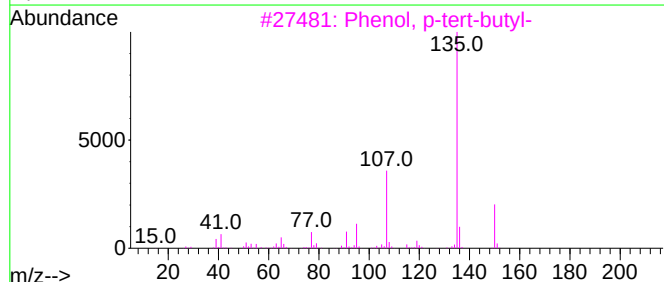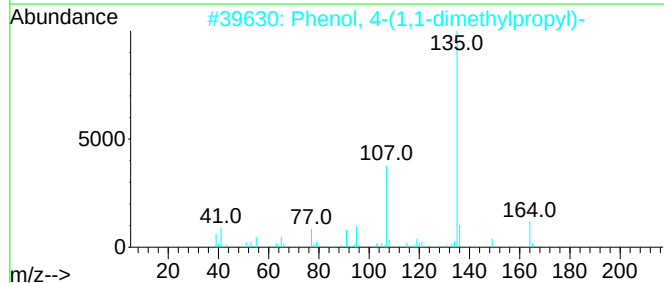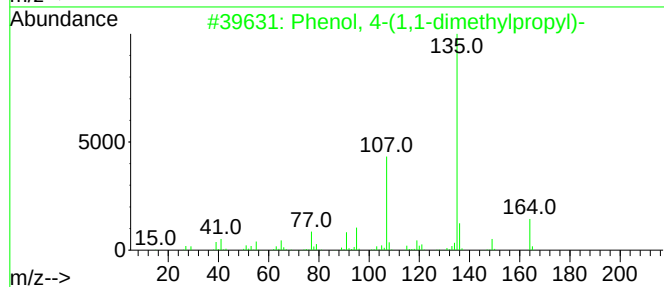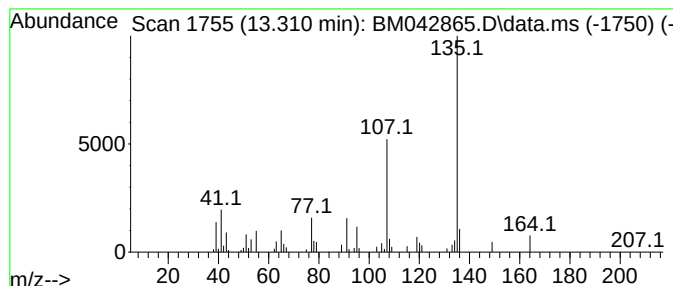

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042865.D
Acq On : 18 Nov 2023 03:59
Operator : MA/JU
Sample : 05226-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, 4-(1,1-...	13.310	5.3	ng/ul	70429	3	14.474	266111	20.0