

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042867.D
 Acq On : 18 Nov 2023 05:49
 Operator : MA/JU
 Sample : PB156892BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK892

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	37	rVB2	11810	16380	1.73%	0.174%
2	3.610	102	106	122	rBV	142249	242264	25.56%	2.572%
3	5.093	356	358	361	rVB3	2043	1501	0.16%	0.016%
4	5.275	387	389	393	rBV3	942	1103	0.12%	0.012%
5	5.404	409	411	413	rBV2	1647	1402	0.15%	0.015%
6	5.669	454	456	460	rBV4	1066	988	0.10%	0.010%
7	6.392	577	579	580	rBV2	1006	955	0.10%	0.010%
8	6.987	674	680	697	rBV	142221	294850	31.11%	3.131%
9	7.169	704	711	728	rBV	122595	225442	23.79%	2.394%
10	7.339	734	740	752	rBV	166006	298222	31.47%	3.167%
11	7.457	758	760	764	rVB5	1686	1861	0.20%	0.020%
12	7.622	787	788	791	rVB2	1490	1032	0.11%	0.011%
13	7.657	791	794	797	rBV3	1383	1811	0.19%	0.019%
14	7.816	815	821	833	rBV	109047	202061	21.32%	2.146%
15	8.022	853	856	858	rBV4	1430	1401	0.15%	0.015%
16	8.057	860	862	866	rBV4	657	994	0.10%	0.011%
17	8.539	938	944	965	rBV	157041	326465	34.45%	3.467%
18	8.675	965	967	970	rVB4	1503	1486	0.16%	0.016%
19	8.916	1005	1008	1009	rBV3	971	983	0.10%	0.010%
20	8.939	1009	1012	1014	rBV3	939	963	0.10%	0.010%
21	9.022	1019	1026	1041	rBV	149433	291719	30.78%	3.098%
22	9.569	1116	1119	1120	rVB3	1000	1027	0.11%	0.011%
23	9.592	1120	1123	1125	rBV3	1083	1412	0.15%	0.015%
24	9.733	1138	1147	1163	rBV	123399	250016	26.38%	2.655%
25	9.904	1174	1176	1179	rVB3	1333	1366	0.14%	0.015%
26	9.992	1189	1191	1195	rVB4	1186	1108	0.12%	0.012%
27	10.257	1229	1236	1257	rBV	146305	320040	33.77%	3.398%
28	10.628	1292	1299	1313	rBV	158536	273553	28.86%	2.905%
29	10.810	1324	1330	1350	rBV2	115000	300879	31.75%	3.195%
30	11.033	1366	1368	1371	rVB2	963	975	0.10%	0.010%
31	11.380	1424	1427	1430	rBV3	889	1061	0.11%	0.011%
32	11.522	1448	1451	1454	rVB3	722	962	0.10%	0.010%
33	11.580	1458	1461	1462	rBV	1289	1191	0.13%	0.013%
34	11.904	1514	1516	1519	rBV3	877	1216	0.13%	0.013%
35	12.263	1573	1577	1578	rBV3	953	1217	0.13%	0.013%
36	12.498	1615	1617	1621	rBV3	650	983	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042867.D
 Acq On : 18 Nov 2023 05:49
 Operator : MA/JU
 Sample : PB156892BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK892

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.321	1753	1757	1763	rVB4	2333	3432	0.36%	0.036%
38	13.698	1818	1821	1826	rVB4	772	1386	0.15%	0.015%
39	13.898	1849	1855	1866	rBV	355933	520228	54.89%	5.524%
40	14.174	1896	1902	1913	rBV	392895	562543	59.36%	5.973%
41	14.474	1947	1953	1965	rBV	237999	343511	36.25%	3.648%
42	14.745	1993	1999	2007	rBV4	29529	96773	10.21%	1.028%
43	15.033	2047	2048	2053	rBV3	877	1374	0.14%	0.015%
44	15.468	2116	2122	2133	rBV	475917	697785	73.63%	7.409%
45	15.621	2142	2148	2160	rBV	107851	199768	21.08%	2.121%
46	15.762	2169	2172	2175	rVB2	1113	1288	0.14%	0.014%
47	15.962	2202	2206	2209	rBV3	848	1508	0.16%	0.016%
48	16.133	2233	2235	2238	rVB2	1042	1024	0.11%	0.011%
49	16.592	2309	2313	2317	rVB3	866	1204	0.13%	0.013%
50	16.874	2359	2361	2364	rBV3	771	962	0.10%	0.010%
51	17.027	2385	2387	2389	rBV2	1449	1429	0.15%	0.015%
52	17.227	2415	2421	2432	rBV	282500	395082	41.69%	4.195%
53	17.327	2432	2438	2454	rVV	490902	727721	76.79%	7.727%
54	17.574	2478	2480	2485	rVB4	894	1334	0.14%	0.014%
55	17.809	2516	2520	2523	rBV3	1254	1567	0.17%	0.017%
56	17.909	2535	2537	2540	rBV2	808	1039	0.11%	0.011%
57	18.151	2576	2578	2581	rVB2	1571	1375	0.15%	0.015%
58	18.362	2611	2614	2616	rBV3	920	1046	0.11%	0.011%
59	18.515	2636	2640	2642	rBV5	1012	1139	0.12%	0.012%
60	18.839	2692	2695	2698	rVB3	1004	1197	0.13%	0.013%
61	19.186	2751	2754	2758	rBV3	4033	4774	0.50%	0.051%
62	19.262	2764	2767	2772	rBV3	3698	6184	0.65%	0.066%
63	19.374	2784	2786	2789	rBV3	1092	1256	0.13%	0.013%
64	19.621	2823	2828	2844	rBV	660473	915167	96.57%	9.718%
65	19.962	2884	2886	2887	rBV2	1572	1075	0.11%	0.011%
66	20.086	2903	2907	2909	rBV4	3373	4811	0.51%	0.051%
67	20.162	2918	2920	2921	rBV2	2084	1392	0.15%	0.015%
68	20.397	2958	2960	2961	rBV2	2603	1771	0.19%	0.019%
69	21.415	3128	3133	3146	rBV	260012	425431	44.89%	4.517%
70	23.615	3500	3507	3523	rBV	454135	947714	100.00%	10.063%
71	23.768	3527	3533	3547	rVB	206257	471410	49.74%	5.006%




Sum of corrected areas: 9417589

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042867.D
Acq On : 18 Nov 2023 05:49
Operator : MA/JU
Sample : PB156892BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

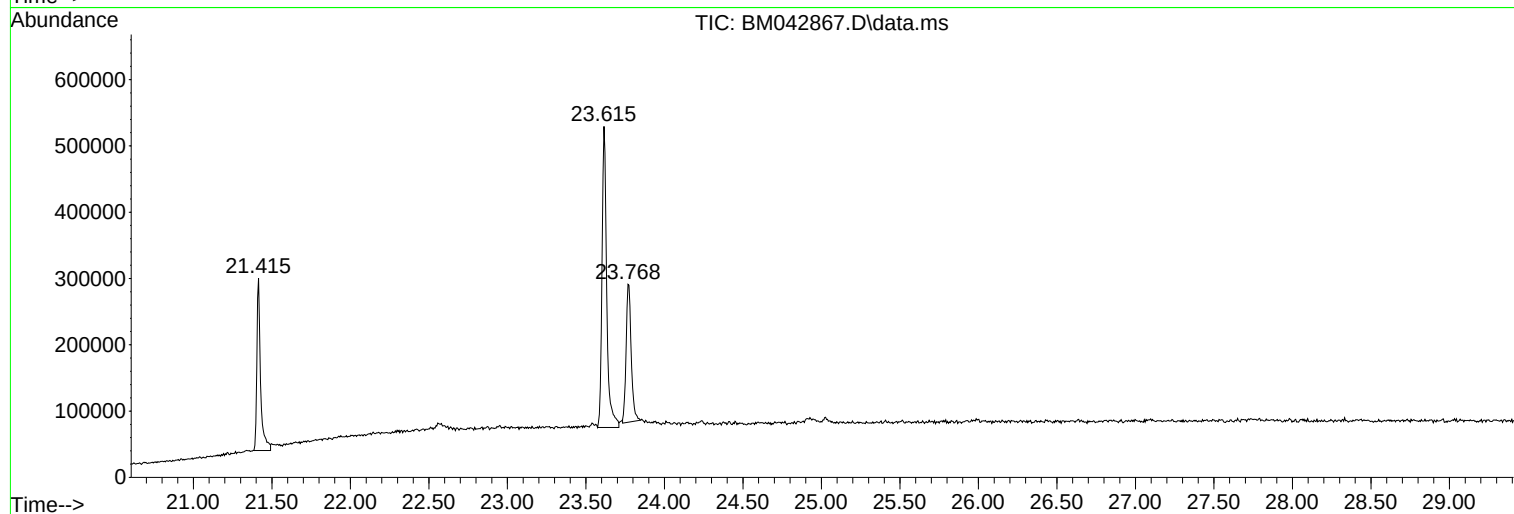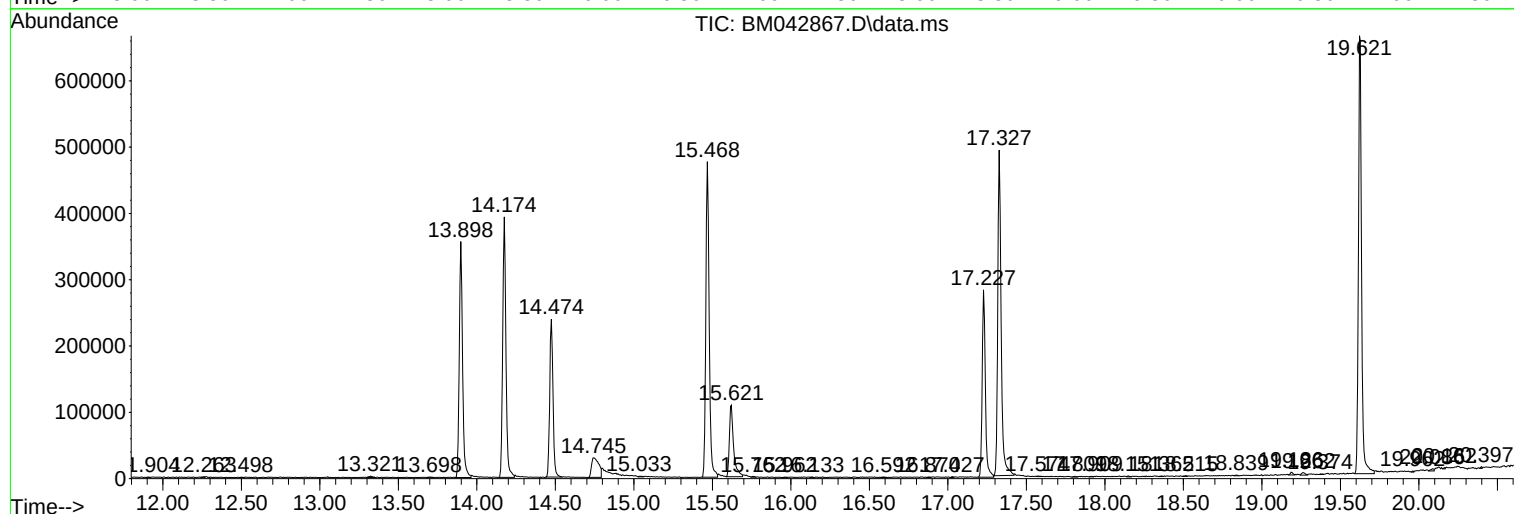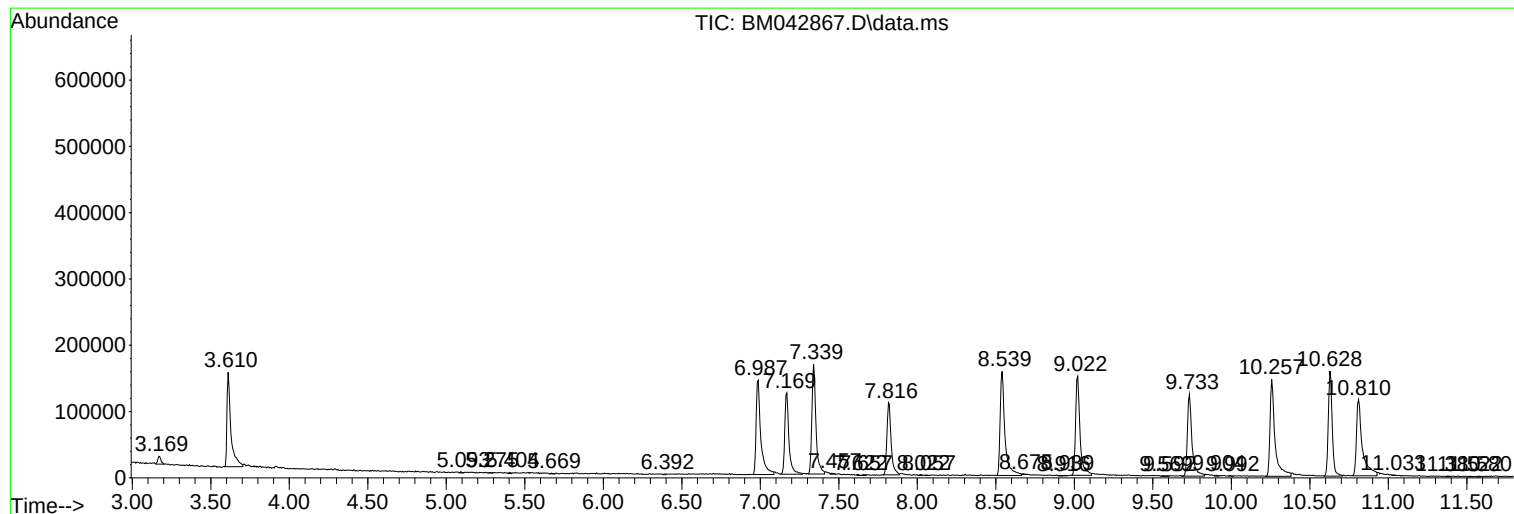

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042867.D
Acq On : 18 Nov 2023 05:49
Operator : MA/JU
Sample : PB156892BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042867.D
Acq On : 18 Nov 2023 05:49
Operator : MA/JU
Sample : PB156892BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc