

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042868.D
 Acq On : 18 Nov 2023 06:26
 Operator : MA/JU
 Sample : PB156975BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK975

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	37	rVB3	13096	17781	1.84%	0.181%
2	3.610	102	106	129	rBV	154523	271398	28.16%	2.769%
3	4.322	225	227	228	rBV2	2208	1741	0.18%	0.018%
4	4.775	302	304	306	rBV2	1464	1323	0.14%	0.013%
5	5.504	426	428	431	rBV4	1203	1282	0.13%	0.013%
6	5.740	466	468	475	rBV5	1273	2993	0.31%	0.031%
7	5.863	485	489	492	rBV5	747	1101	0.11%	0.011%
8	5.922	498	499	504	rBV4	1721	3030	0.31%	0.031%
9	6.340	568	570	572	rBV2	1267	1187	0.12%	0.012%
10	6.481	592	594	596	rBV3	1781	1461	0.15%	0.015%
11	6.981	674	679	699	rVV	155868	318386	33.03%	3.248%
12	7.163	705	710	728	rVB	128351	232408	24.11%	2.371%
13	7.340	734	740	760	rVV	182688	325762	33.80%	3.323%
14	7.463	760	761	764	rVV3	1673	1611	0.17%	0.016%
15	7.510	767	769	771	rVB3	1200	1082	0.11%	0.011%
16	7.534	771	773	777	rVB2	1020	1189	0.12%	0.012%
17	7.616	785	787	789	rBV2	1518	1334	0.14%	0.014%
18	7.698	800	801	804	rVB3	1108	1034	0.11%	0.011%
19	7.816	815	821	836	rVV	112808	210478	21.84%	2.147%
20	8.004	851	853	856	rVB3	826	1003	0.10%	0.010%
21	8.069	861	864	869	rBV5	822	1690	0.18%	0.017%
22	8.539	938	944	959	rBV	176505	334102	34.66%	3.408%
23	8.969	1014	1017	1018	rBV2	1259	1243	0.13%	0.013%
24	9.022	1019	1026	1039	rBV	162632	305932	31.74%	3.121%
25	9.734	1140	1147	1164	rBV	134767	266962	27.70%	2.724%
26	9.881	1170	1172	1174	rVB3	1467	1001	0.10%	0.010%
27	10.257	1230	1236	1252	rBV2	157972	329244	34.16%	3.359%
28	10.428	1264	1265	1275	rVB5	1293	2690	0.28%	0.027%
29	10.628	1293	1299	1313	rBV	156760	267526	27.76%	2.729%
30	10.810	1323	1330	1354	rBV	126975	330773	34.32%	3.375%
31	11.010	1362	1364	1366	rVB3	1274	1062	0.11%	0.011%
32	11.151	1385	1388	1391	rVB2	997	1208	0.13%	0.012%
33	11.498	1442	1447	1448	rBV4	905	1248	0.13%	0.013%
34	12.180	1558	1563	1564	rVB3	783	1064	0.11%	0.011%
35	13.557	1792	1797	1800	rBV3	728	1110	0.12%	0.011%
36	13.898	1849	1855	1869	rBV	367530	536313	55.64%	5.471%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042868.D
 Acq On : 18 Nov 2023 06:26
 Operator : MA/JU
 Sample : PB156975BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK975

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.986	1869	1870	1873	rVB2	1130	974	0.10%	0.010%
38	14.174	1895	1902	1911	rBV	399425	583209	60.51%	5.950%
39	14.474	1947	1953	1965	rBV	234866	341402	35.42%	3.483%
40	14.739	1992	1998	2020	rBV5	32856	150662	15.63%	1.537%
41	15.468	2116	2122	2136	rBV	501221	734484	76.21%	7.493%
42	15.615	2142	2147	2162	rBV	121963	209857	21.77%	2.141%
43	15.710	2162	2163	2171	rVB5	3787	3852	0.40%	0.039%
44	16.274	2256	2259	2263	rBV2	714	1082	0.11%	0.011%
45	16.404	2275	2281	2282	rBV2	751	1021	0.11%	0.010%
46	16.504	2293	2298	2300	rBV3	1171	1843	0.19%	0.019%
47	16.598	2311	2314	2318	rVB2	1035	1247	0.13%	0.013%
48	16.762	2338	2342	2344	rVB2	1012	1245	0.13%	0.013%
49	16.792	2344	2347	2351	rBV3	1048	1880	0.20%	0.019%
50	17.227	2415	2421	2432	rBV	267553	392620	40.74%	4.005%
51	17.327	2432	2438	2456	rVV	517063	769298	79.82%	7.848%
52	17.939	2539	2542	2543	rVV2	1110	1028	0.11%	0.010%
53	17.974	2547	2548	2553	rBV2	1097	1524	0.16%	0.016%
54	18.351	2607	2612	2614	rVB4	994	1500	0.16%	0.015%
55	18.468	2629	2632	2635	rBV4	609	969	0.10%	0.010%
56	18.509	2637	2639	2641	rVV2	1204	1222	0.13%	0.012%
57	18.756	2677	2681	2683	rBV3	1116	1456	0.15%	0.015%
58	18.821	2690	2692	2695	rBV3	1208	1482	0.15%	0.015%
59	18.845	2695	2696	2700	rVV2	1193	967	0.10%	0.010%
60	19.062	2731	2733	2738	rBV5	662	983	0.10%	0.010%
61	19.145	2746	2747	2750	rBV4	1151	1080	0.11%	0.011%
62	19.186	2750	2754	2758	rBV5	4399	6081	0.63%	0.062%
63	19.262	2765	2767	2772	rVV5	3146	4067	0.42%	0.041%
64	19.392	2786	2789	2792	rBV4	1572	2031	0.21%	0.021%
65	19.439	2794	2797	2800	rVV3	1158	1772	0.18%	0.018%
66	19.621	2823	2828	2844	rVV	682668	950311	98.60%	9.695%
67	19.974	2887	2888	2891	rBV3	2460	2698	0.28%	0.028%
68	20.574	2989	2990	2992	rBV2	2628	1544	0.16%	0.016%
69	21.415	3128	3133	3144	rBV	265577	413302	42.88%	4.216%
70	23.615	3500	3507	3520	rBV	477589	963814	100.00%	9.833%
71	23.768	3527	3533	3547	rVB	224553	468795	48.64%	4.783%




Sum of corrected areas: 9802054

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042868.D
Acq On : 18 Nov 2023 06:26
Operator : MA/JU
Sample : PB156975BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

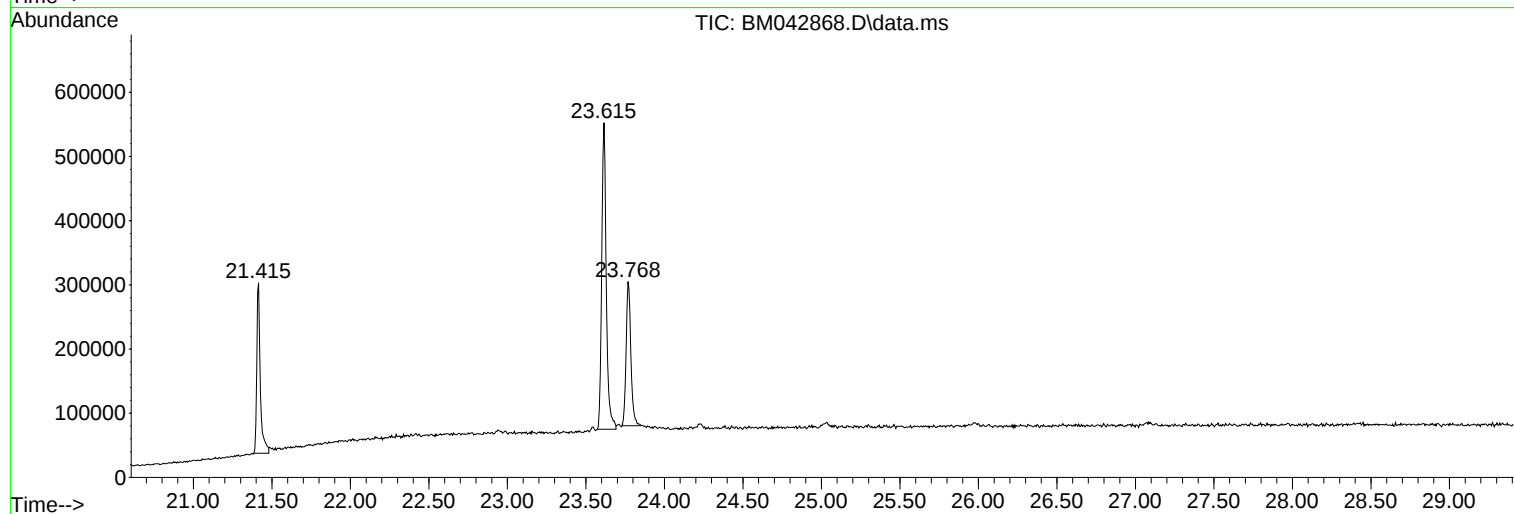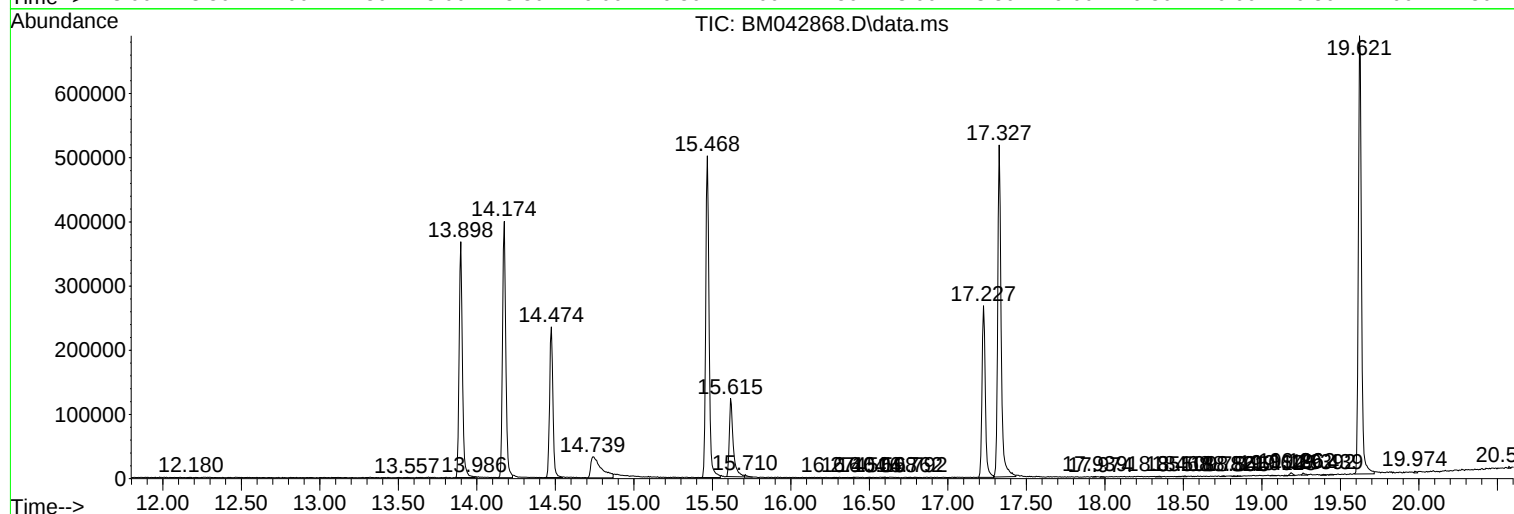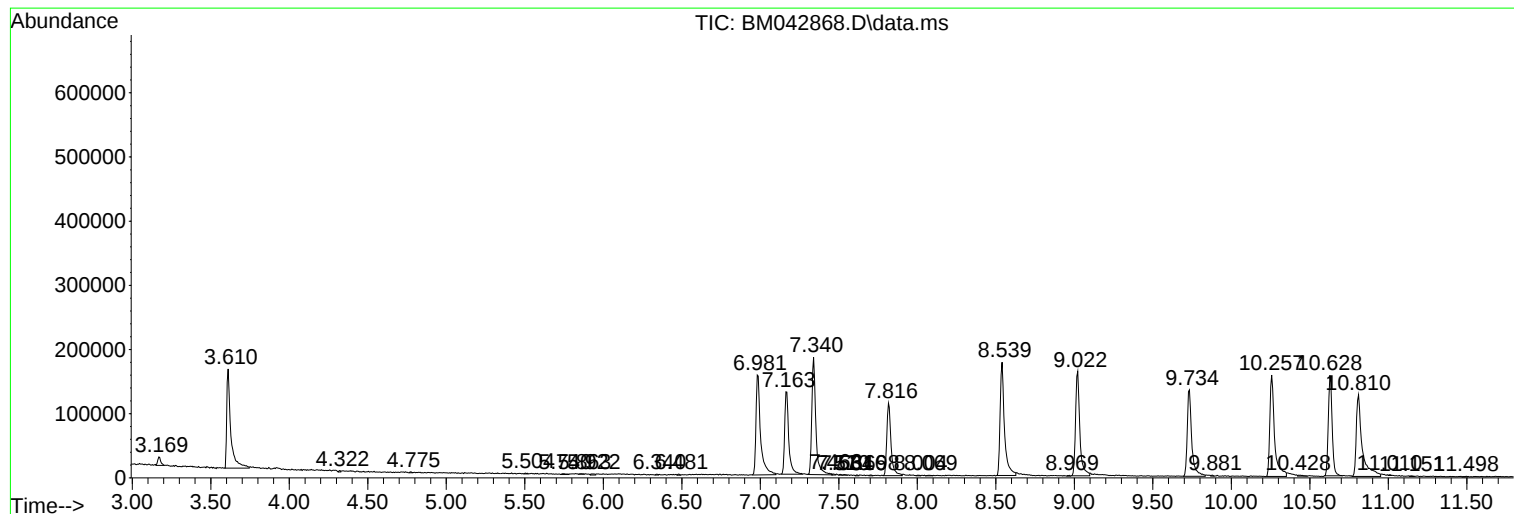

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042868.D
Acq On : 18 Nov 2023 06:26
Operator : MA/JU
Sample : PB156975BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042868.D
Acq On : 18 Nov 2023 06:26
Operator : MA/JU
Sample : PB156975BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------