

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042869.D
 Acq On : 18 Nov 2023 07:02
 Operator : MA/JU
 Sample : PB156976BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	37	rVB2	11830	14991	1.92%	0.182%
2	3.610	103	106	119	rBV	131655	218853	28.09%	2.661%
3	3.916	154	158	163	rBV3	3782	6127	0.79%	0.074%
4	4.046	179	180	182	rBV2	2030	1463	0.19%	0.018%
5	4.216	207	209	211	rBV3	1800	1050	0.13%	0.013%
6	4.534	261	263	266	rVB3	1411	922	0.12%	0.011%
7	4.593	271	273	274	rBV2	1854	952	0.12%	0.012%
8	4.875	319	321	324	rBV3	1697	1264	0.16%	0.015%
9	5.028	345	347	348	rBV2	1136	1017	0.13%	0.012%
10	5.075	354	355	356	rBV	1570	975	0.13%	0.012%
11	5.110	359	361	363	rBV3	1289	1067	0.14%	0.013%
12	5.499	425	427	430	rVB3	1097	1122	0.14%	0.014%
13	5.652	451	453	455	rVB2	1126	859	0.11%	0.010%
14	5.728	465	466	470	rBV4	978	1122	0.14%	0.014%
15	5.799	476	478	479	rVB2	1288	822	0.11%	0.010%
16	6.040	517	519	521	rVB2	1496	1125	0.14%	0.014%
17	6.057	521	522	525	rBV3	1771	1108	0.14%	0.013%
18	6.269	556	558	561	rVB4	1327	1144	0.15%	0.014%
19	6.340	567	570	571	rBV3	1062	1228	0.16%	0.015%
20	6.469	590	592	594	rVB2	1006	929	0.12%	0.011%
21	6.540	602	604	606	rBV2	1082	1168	0.15%	0.014%
22	6.640	619	621	622	rBV2	1353	818	0.10%	0.010%
23	6.657	622	624	626	rVV3	926	974	0.13%	0.012%
24	6.699	629	631	634	rVB4	1087	912	0.12%	0.011%
25	6.781	644	645	648	rVB3	1214	971	0.12%	0.012%
26	6.981	674	679	693	rBV	127211	257984	33.11%	3.137%
27	7.163	705	710	721	rBV	108580	190080	24.40%	2.311%
28	7.340	734	740	758	rVV	148568	270217	34.68%	3.286%
29	7.475	761	763	765	rVV3	1201	897	0.12%	0.011%
30	7.498	765	767	769	rVB2	1306	1266	0.16%	0.015%
31	7.816	815	821	838	rBV	110179	206815	26.54%	2.515%
32	8.169	878	881	883	rBV4	1101	1189	0.15%	0.014%
33	8.340	907	910	913	rVB3	1027	1146	0.15%	0.014%
34	8.540	938	944	964	rBV	136328	283335	36.36%	3.445%
35	8.692	969	970	975	rVB3	2109	1753	0.22%	0.021%
36	8.945	1012	1013	1017	rVB3	1000	916	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042869.D
 Acq On : 18 Nov 2023 07:02
 Operator : MA/JU
 Sample : PB156976BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	9.022	1017	1026	1039	rBV	127382	256335	32.90%	3.117%
38	9.734	1141	1147	1166	rBV	105736	214315	27.51%	2.606%
39	9.892	1172	1174	1176	rVB3	1162	957	0.12%	0.012%
40	9.916	1176	1178	1183	rVB6	1228	1685	0.22%	0.020%
41	9.987	1186	1190	1191	rBV3	1140	1090	0.14%	0.013%
42	10.257	1228	1236	1255	rBV	124052	273725	35.13%	3.328%
43	10.392	1257	1259	1261	rVB2	1745	1418	0.18%	0.017%
44	10.628	1293	1299	1314	rVV	154692	266915	34.26%	3.245%
45	10.810	1324	1330	1344	rBV	97145	240240	30.83%	2.921%
46	10.992	1359	1361	1364	rVB3	1163	1229	0.16%	0.015%
47	11.057	1370	1372	1376	rVB4	943	952	0.12%	0.012%
48	11.322	1414	1417	1420	rBV2	723	1198	0.15%	0.015%
49	11.704	1479	1482	1486	rBV4	763	1007	0.13%	0.012%
50	11.781	1493	1495	1499	rBV3	751	1143	0.15%	0.014%
51	12.269	1574	1578	1581	rBV5	1028	1680	0.22%	0.020%
52	12.504	1615	1618	1619	rVB3	1047	868	0.11%	0.011%
53	12.522	1619	1621	1623	rBV3	804	788	0.10%	0.010%
54	13.322	1753	1757	1762	rVB3	1905	2836	0.36%	0.034%
55	13.692	1818	1820	1824	rVB4	1063	1049	0.13%	0.013%
56	13.898	1849	1855	1873	rBV	290891	431582	55.39%	5.248%
57	14.174	1895	1902	1910	rBV	320205	469794	60.30%	5.712%
58	14.474	1947	1953	1962	rBV	222183	321992	41.33%	3.915%
59	14.627	1975	1979	1980	rBV3	854	1009	0.13%	0.012%
60	14.757	1992	2001	2022	rBV6	21624	107394	13.78%	1.306%
61	14.957	2033	2035	2042	rVB5	846	1440	0.18%	0.018%
62	15.039	2048	2049	2054	rVB4	1239	1607	0.21%	0.020%
63	15.086	2054	2057	2058	rBV2	1188	896	0.11%	0.011%
64	15.145	2063	2067	2070	rBV4	536	815	0.10%	0.010%
65	15.233	2079	2082	2085	rBV3	989	1148	0.15%	0.014%
66	15.257	2085	2086	2091	rVV2	762	1176	0.15%	0.014%
67	15.404	2108	2111	2113	rBV4	661	942	0.12%	0.011%
68	15.469	2116	2122	2140	rVV	374638	587625	75.42%	7.145%
69	15.616	2142	2147	2168	rVV	82755	165038	21.18%	2.007%
70	15.751	2168	2170	2175	rVV3	1166	2200	0.28%	0.027%
71	16.504	2295	2298	2301	rBV2	872	1136	0.15%	0.014%
72	16.633	2317	2320	2323	rBV3	681	1126	0.14%	0.014%
73	16.957	2372	2375	2379	rVB2	536	789	0.10%	0.010%
74	17.021	2384	2386	2390	rVV2	1217	829	0.11%	0.010%
75	17.227	2415	2421	2432	rBV	257956	364924	46.84%	4.437%
76	17.327	2432	2438	2453	rBV	394839	605888	77.76%	7.367%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042869.D
 Acq On : 18 Nov 2023 07:02
 Operator : MA/JU
 Sample : PB156976BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

77	17.539	2471	2474	2476	rVB3	859	866	0.11%	0.011%
78	17.751	2508	2510	2512	rVB2	1291	914	0.12%	0.011%
79	17.792	2512	2517	2520	rBV5	1150	1607	0.21%	0.020%
80	17.857	2527	2528	2532	rVB3	869	796	0.10%	0.010%
81	18.386	2615	2618	2621	rBV3	737	974	0.13%	0.012%
82	18.504	2636	2638	2642	rVB4	1408	1280	0.16%	0.016%
83	18.568	2648	2649	2653	rBV3	806	1209	0.16%	0.015%
84	18.662	2662	2665	2667	rVB3	1155	978	0.13%	0.012%
85	18.692	2667	2670	2671	rBV2	857	885	0.11%	0.011%
86	18.786	2684	2686	2688	rBV3	817	794	0.10%	0.010%
87	18.827	2690	2693	2695	rBV3	964	981	0.13%	0.012%
88	18.857	2695	2698	2699	rBV2	1144	1204	0.15%	0.015%
89	18.998	2720	2722	2724	rVB2	946	806	0.10%	0.010%
90	19.015	2724	2725	2728	rVB3	1041	955	0.12%	0.012%
91	19.192	2751	2755	2758	rBV3	3571	4572	0.59%	0.056%
92	19.257	2764	2766	2769	rBV3	2617	2880	0.37%	0.035%
93	19.468	2799	2802	2805	rBV5	1011	1485	0.19%	0.018%
94	19.621	2823	2828	2846	rBV	545247	759591	97.49%	9.236%
95	19.774	2852	2854	2855	rBV2	1518	1112	0.14%	0.014%
96	20.180	2921	2923	2926	rBV3	1706	1888	0.24%	0.023%
97	20.209	2926	2928	2930	rBV3	2127	1906	0.24%	0.023%
98	21.415	3128	3133	3145	rBV	239311	389889	50.04%	4.741%
99	23.615	3500	3507	3520	rBV	381291	779157	100.00%	9.474%
100	23.768	3527	3533	3546	rBV	216541	450277	57.79%	5.475%




Sum of corrected areas: 8224367

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042869.D
Acq On : 18 Nov 2023 07:02
Operator : MA/JU
Sample : PB156976BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

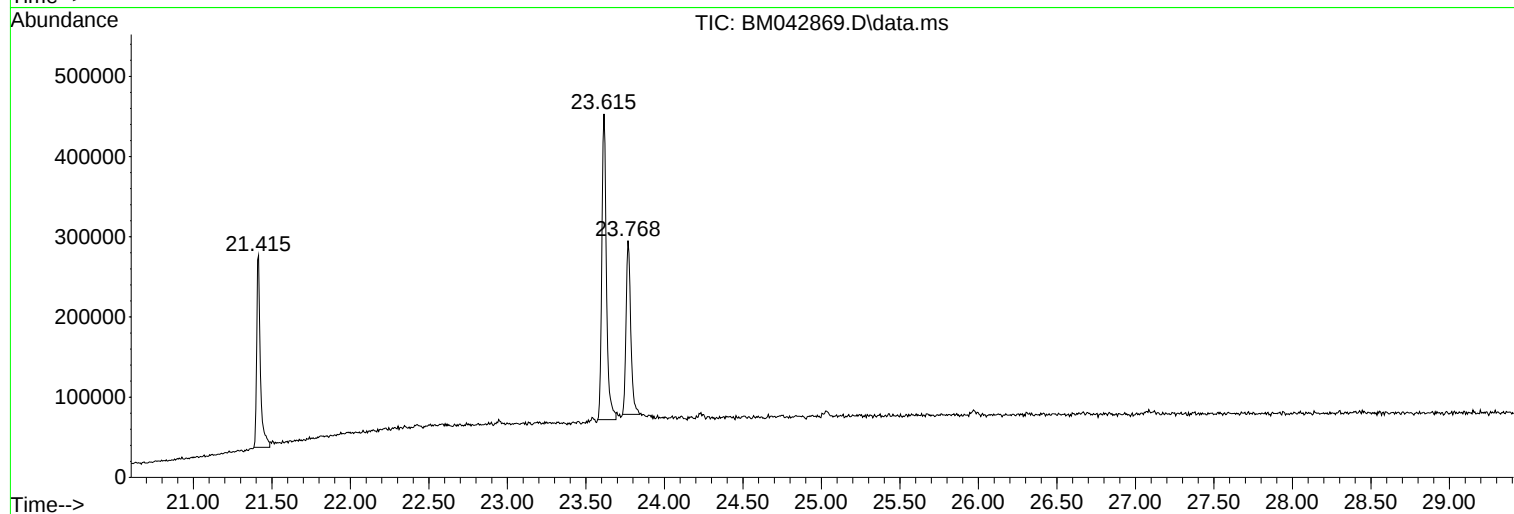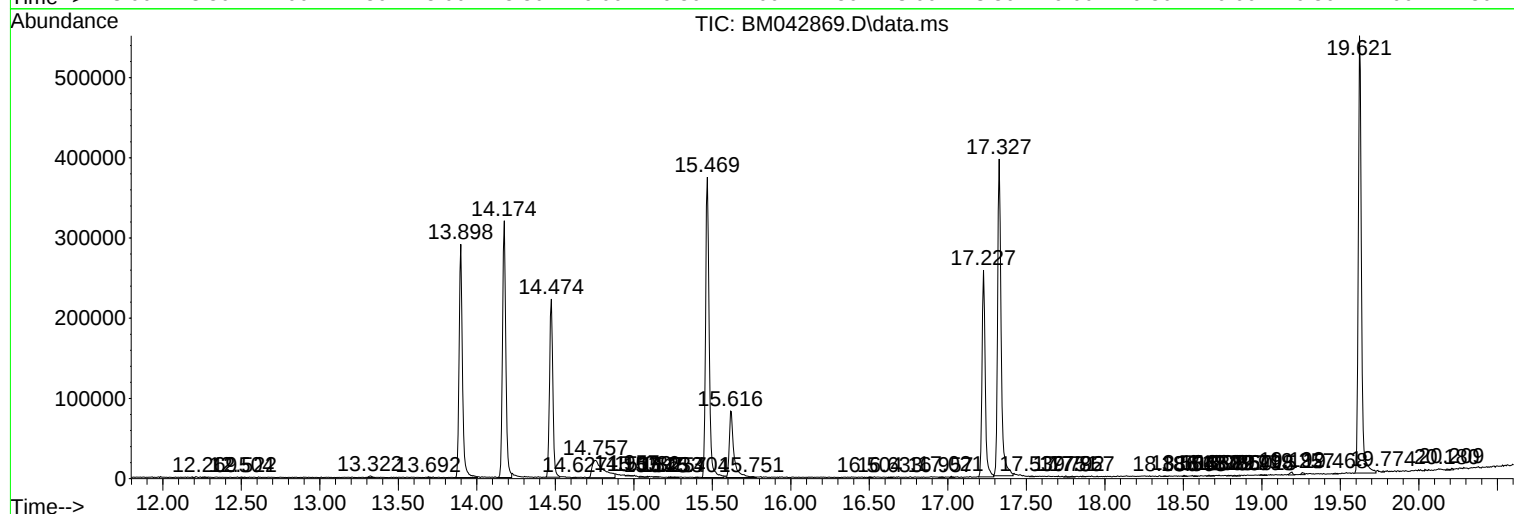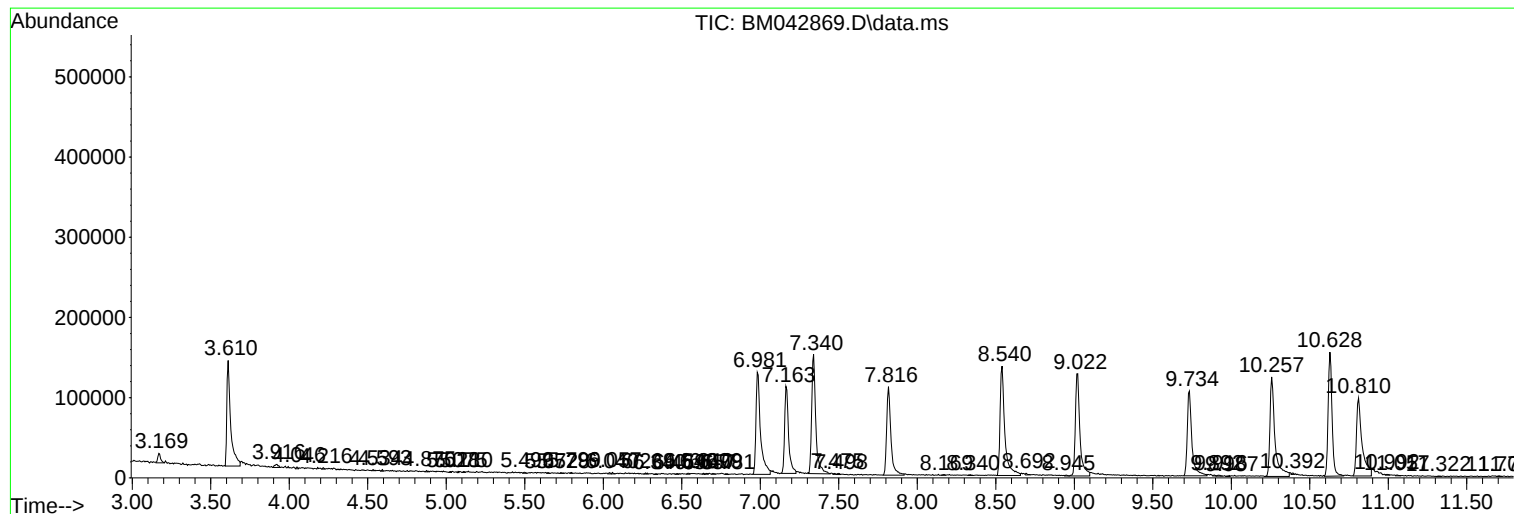

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042869.D
Acq On : 18 Nov 2023 07:02
Operator : MA/JU
Sample : PB156976BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042869.D
Acq On : 18 Nov 2023 07:02
Operator : MA/JU
Sample : PB156976BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------