

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042873.D
 Acq On : 18 Nov 2023 09:27
 Operator : MA/JU
 Sample : 05226-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	37	rVB3	8662	11232	1.09%	0.140%
2	3.616	104	107	125	rBV	34005	75660	7.36%	0.944%
3	3.910	155	157	159	rBV3	2360	2138	0.21%	0.027%
4	4.481	252	254	257	rBV3	1224	1414	0.14%	0.018%
5	4.681	286	288	291	rBV2	1141	1471	0.14%	0.018%
6	5.016	341	345	346	rBV4	1557	1649	0.16%	0.021%
7	5.093	356	358	360	rBV3	1255	1144	0.11%	0.014%
8	5.116	360	362	364	rVB2	1466	1113	0.11%	0.014%
9	5.551	434	436	441	rVB5	1058	1066	0.10%	0.013%
10	5.875	489	491	497	rVB5	1037	1438	0.14%	0.018%
11	5.916	497	498	501	rBV3	1405	1094	0.11%	0.014%
12	5.975	506	508	512	rBV4	686	1155	0.11%	0.014%
13	6.128	532	534	535	rBV	1270	1046	0.10%	0.013%
14	6.410	578	582	583	rBV4	1202	1236	0.12%	0.015%
15	6.463	588	591	595	rVB5	1018	1587	0.15%	0.020%
16	6.722	632	635	638	rBV3	1136	1243	0.12%	0.016%
17	6.992	677	681	694	rBV5	13994	41843	4.07%	0.522%
18	7.163	705	710	728	rBV	113188	209628	20.40%	2.617%
19	7.339	734	740	758	rBV	110075	206171	20.07%	2.573%
20	7.587	780	782	785	rVB4	1246	1317	0.13%	0.016%
21	7.816	815	821	831	rBV	83249	158760	15.45%	1.982%
22	7.981	847	849	852	rVB4	1063	1324	0.13%	0.017%
23	8.263	893	897	900	rVB3	882	1147	0.11%	0.014%
24	8.545	938	945	963	rBV	54646	128212	12.48%	1.600%
25	9.016	1019	1025	1040	rBV	138244	276543	26.92%	3.452%
26	9.645	1130	1132	1134	rBV2	1081	1123	0.11%	0.014%
27	9.728	1141	1146	1167	rBV	112108	226227	22.02%	2.824%
28	9.869	1169	1170	1176	rVV5	1559	1944	0.19%	0.024%
29	9.922	1176	1179	1181	rVB4	1048	1258	0.12%	0.016%
30	10.257	1230	1236	1254	rBV	116275	262953	25.59%	3.282%
31	10.433	1264	1266	1269	rVB4	1037	1126	0.11%	0.014%
32	10.627	1292	1299	1314	rBV	117552	209076	20.35%	2.610%
33	10.739	1316	1318	1322	rVB3	984	1087	0.11%	0.014%
34	10.810	1324	1330	1351	rBV	84045	231744	22.56%	2.893%
35	11.692	1477	1480	1485	rVB5	1291	2091	0.20%	0.026%
36	12.151	1555	1558	1561	rBV3	1182	1139	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042873.D
 Acq On : 18 Nov 2023 09:27
 Operator : MA/JU
 Sample : 05226-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	12.551	1623	1626	1630	rBV3	998	1306	0.13%	0.016%
38	13.316	1752	1756	1761	rBV4	3051	4994	0.49%	0.062%
39	13.898	1849	1855	1877	rBV	304574	469877	45.74%	5.865%
40	14.174	1895	1902	1913	rBV	352816	525007	51.10%	6.553%
41	14.474	1947	1953	1965	rBV	163367	254515	24.77%	3.177%
42	14.821	2010	2012	2016	rVV3	1019	1682	0.16%	0.021%
43	14.863	2016	2019	2022	rVB3	932	1180	0.11%	0.015%
44	14.980	2036	2039	2042	rVB4	949	1030	0.10%	0.013%
45	15.080	2052	2056	2058	rBV2	1032	1563	0.15%	0.020%
46	15.468	2116	2122	2138	rBV	442432	662121	64.45%	8.265%
47	15.615	2142	2147	2159	rBV2	97055	178653	17.39%	2.230%
48	15.774	2170	2174	2179	rVB4	1057	1514	0.15%	0.019%
49	16.333	2266	2269	2271	rBV	972	1036	0.10%	0.013%
50	16.574	2307	2310	2313	rBV3	1038	1039	0.10%	0.013%
51	17.039	2385	2389	2392	rVB3	1053	1557	0.15%	0.019%
52	17.227	2415	2421	2432	rBV	204661	299877	29.19%	3.743%
53	17.327	2432	2438	2455	rVV	486867	750226	73.02%	9.364%
54	17.868	2528	2530	2533	rVB4	1361	1084	0.11%	0.014%
55	17.892	2533	2534	2539	rBV4	1408	1803	0.18%	0.023%
56	18.086	2562	2567	2576	rVB5	4271	7115	0.69%	0.089%
57	18.321	2604	2607	2608	rVB3	1123	1153	0.11%	0.014%
58	18.351	2608	2612	2613	rBV3	919	1257	0.12%	0.016%
59	18.362	2613	2614	2617	rVV3	1357	1579	0.15%	0.020%
60	18.409	2620	2622	2626	rVB4	1093	1353	0.13%	0.017%
61	18.521	2637	2641	2644	rBV6	1367	2307	0.22%	0.029%
62	18.650	2661	2663	2666	rVB4	1076	1105	0.11%	0.014%
63	19.133	2743	2745	2748	rBV3	1075	1205	0.12%	0.015%
64	19.186	2750	2754	2756	rBV2	4854	5568	0.54%	0.070%
65	19.262	2763	2767	2773	rBV3	3710	5309	0.52%	0.066%
66	19.368	2781	2785	2789	rBV6	2973	4974	0.48%	0.062%
67	19.403	2789	2791	2792	rVB2	2014	1224	0.12%	0.015%
68	19.421	2792	2794	2796	rBV2	1335	1436	0.14%	0.018%
69	19.621	2823	2828	2844	rBV	738989	973496	94.76%	12.151%
70	19.862	2867	2869	2870	rBV2	1778	1703	0.17%	0.021%
71	19.980	2887	2889	2891	rBV3	1959	2398	0.23%	0.030%
72	21.415	3128	3133	3143	rBV	208341	334850	32.59%	4.180%
73	23.615	3500	3507	3520	rBV	521953	1027378	100.00%	12.824%
74	23.768	3527	3533	3546	rVB	188108	405625	39.48%	5.063%

Sum of corrected areas: 8011498

Instrument :

BNA_M

ClientSampleId :




YCG43

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042873.D
Acq On : 18 Nov 2023 09:27
Operator : MA/JU
Sample : 05226-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

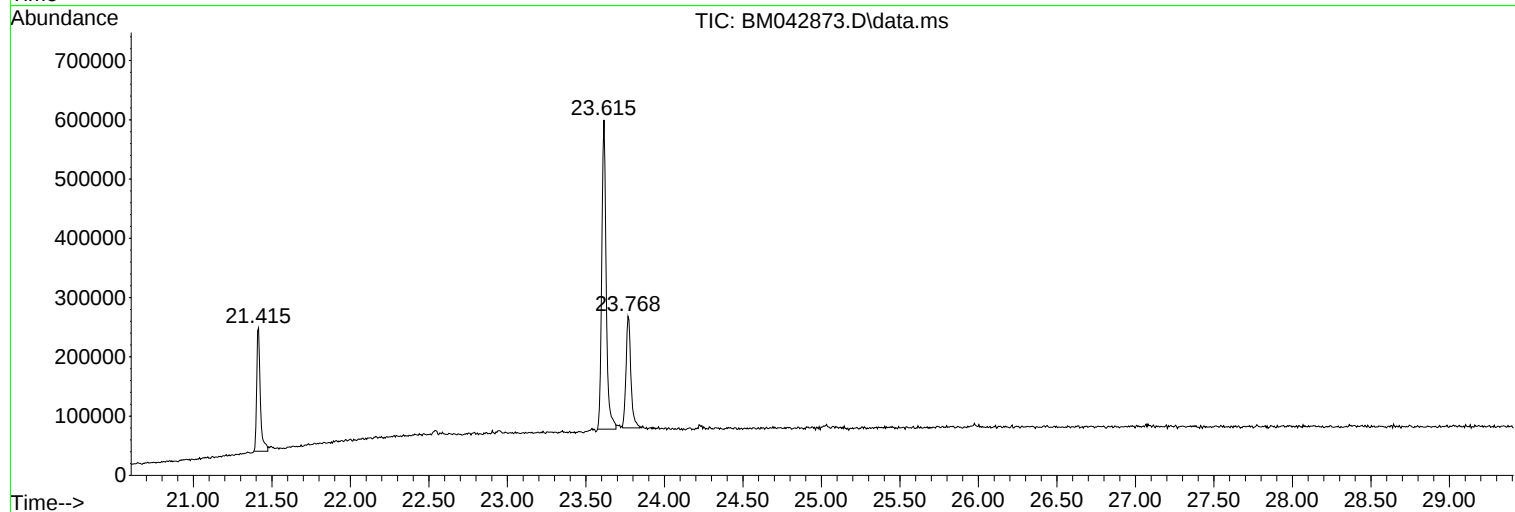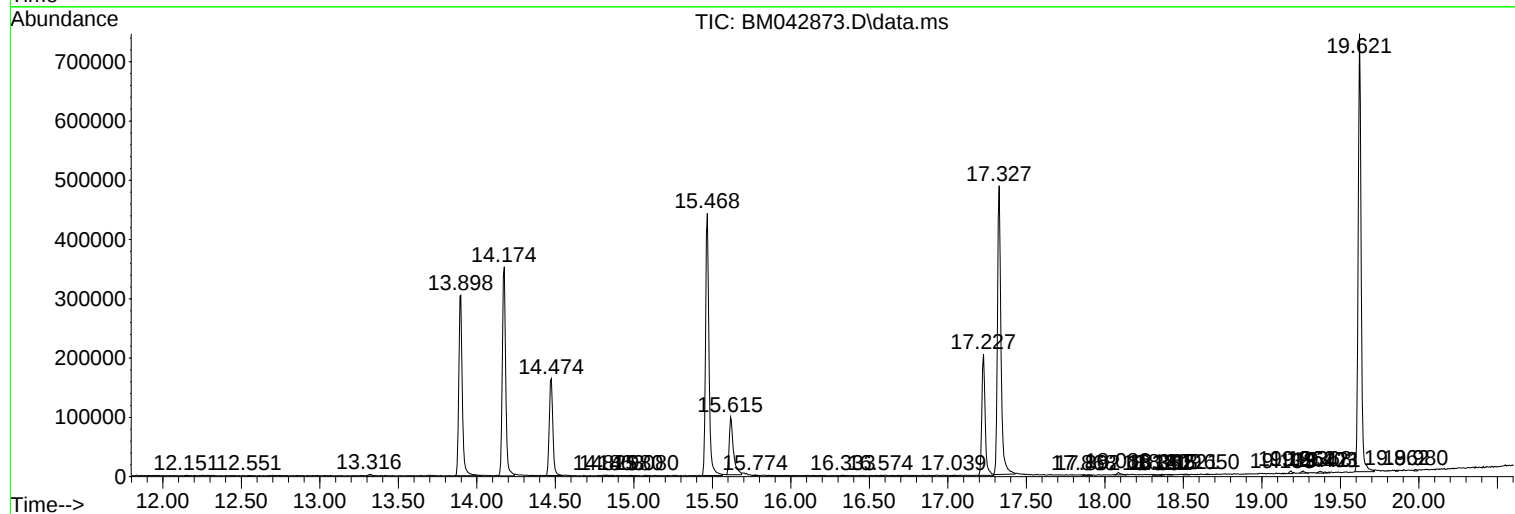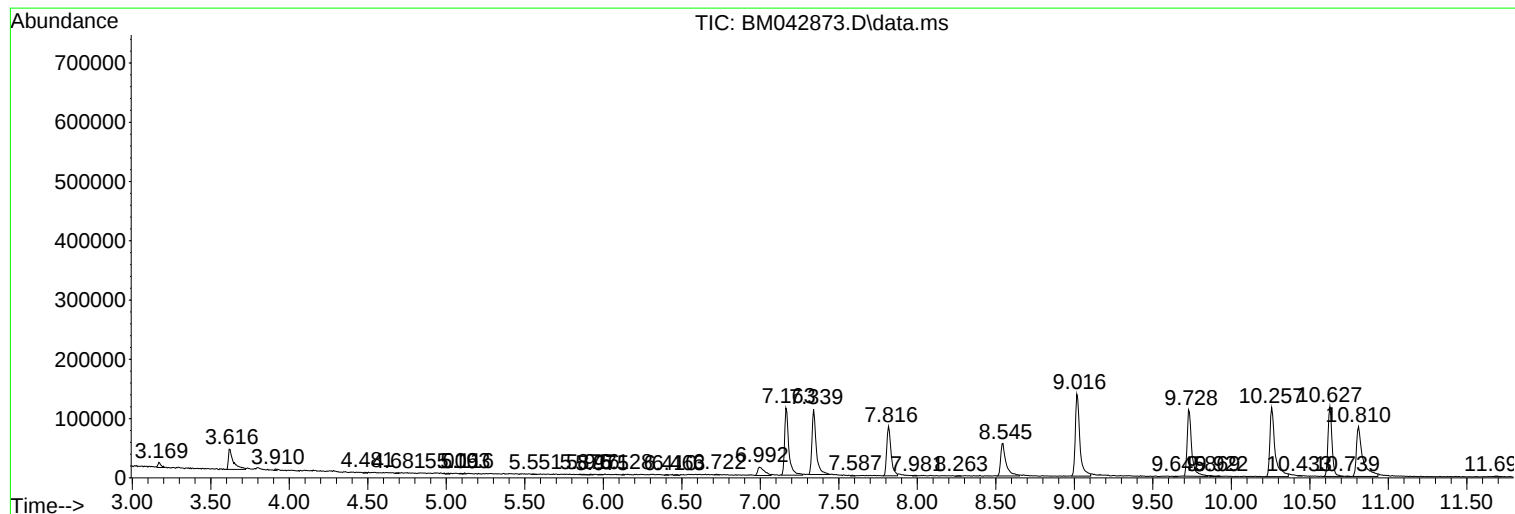

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042873.D
Acq On : 18 Nov 2023 09:27
Operator : MA/JU
Sample : 05226-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042873.D
Acq On : 18 Nov 2023 09:27
Operator : MA/JU
Sample : 05226-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG43

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc