

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042874.D
 Acq On : 18 Nov 2023 10:03
 Operator : MA/JU
 Sample : 05226-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCGB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	41	rVB4	10777	15786	1.62%	0.181%
2	3.622	105	108	118	rBV	27512	53557	5.50%	0.613%
3	3.916	155	158	163	rVB5	3290	5018	0.52%	0.057%
4	4.522	259	261	265	rBV5	1428	1181	0.12%	0.014%
5	4.604	274	275	277	rBV2	1457	1265	0.13%	0.014%
6	4.704	290	292	293	rBV	1570	1082	0.11%	0.012%
7	4.922	325	329	332	rBV6	2270	2808	0.29%	0.032%
8	5.157	366	369	370	rBV3	1360	1376	0.14%	0.016%
9	5.363	402	404	405	rBV	1533	1348	0.14%	0.015%
10	5.510	427	429	432	rBV2	1294	1494	0.15%	0.017%
11	5.969	505	507	509	rBV3	1184	1057	0.11%	0.012%
12	6.551	604	606	610	rBV4	1063	1141	0.12%	0.013%
13	6.787	645	646	650	rBV4	1126	1389	0.14%	0.016%
14	6.916	666	668	670	rVB2	1218	1059	0.11%	0.012%
15	6.992	677	681	692	rBV3	13660	35635	3.66%	0.408%
16	7.069	692	694	697	rVB4	1581	1227	0.13%	0.014%
17	7.163	705	710	727	rBV	103839	194444	19.97%	2.227%
18	7.340	735	740	752	rBV	100739	189064	19.41%	2.165%
19	7.816	815	821	835	rVV	156732	279185	28.67%	3.197%
20	7.945	841	843	846	rBV4	1007	1041	0.11%	0.012%
21	8.539	938	944	956	rBV2	49965	110369	11.33%	1.264%
22	8.945	1010	1013	1016	rVB3	799	1053	0.11%	0.012%
23	9.016	1019	1025	1041	rBV	128553	255562	26.24%	2.927%
24	9.498	1106	1107	1113	rVB4	1133	1220	0.13%	0.014%
25	9.557	1115	1117	1120	rBV3	856	1055	0.11%	0.012%
26	9.728	1140	1146	1160	rBV	99340	198214	20.35%	2.270%
27	9.986	1188	1190	1194	rVB4	842	978	0.10%	0.011%
28	10.257	1230	1236	1255	rBV	104123	236679	24.30%	2.711%
29	10.628	1292	1299	1313	rBV	202192	352796	36.22%	4.040%
30	10.739	1316	1318	1321	rVB2	1244	1100	0.11%	0.013%
31	10.810	1324	1330	1353	rVV2	63831	194154	19.94%	2.223%
32	10.980	1357	1359	1361	rVV3	2516	2608	0.27%	0.030%
33	11.175	1390	1392	1397	rVB4	778	1200	0.12%	0.014%
34	11.292	1409	1412	1415	rVB4	1166	1024	0.11%	0.012%
35	13.051	1706	1711	1717	rVB4	704	1781	0.18%	0.020%
36	13.316	1751	1756	1761	rBV4	2865	4257	0.44%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042874.D
 Acq On : 18 Nov 2023 10:03
 Operator : MA/JU
 Sample : 05226-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCGB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.892	1849	1854	1868	rBV	276958	426803	43.82%	4.888%
38	14.010	1873	1874	1878	rVB3	1092	1077	0.11%	0.012%
39	14.174	1895	1902	1910	rBV	320236	475680	48.84%	5.448%
40	14.257	1914	1916	1919	rVB3	1167	1219	0.13%	0.014%
41	14.474	1946	1953	1965	rBV	289179	442488	45.43%	5.067%
42	14.592	1971	1973	1978	rVB3	900	1071	0.11%	0.012%
43	14.880	2020	2022	2025	rVB2	996	1034	0.11%	0.012%
44	15.468	2116	2122	2135	rBV	401122	609284	62.56%	6.978%
45	15.621	2142	2148	2159	rBV2	83900	159713	16.40%	1.829%
46	15.715	2162	2164	2172	rVV4	3005	5434	0.56%	0.062%
47	16.110	2227	2231	2234	rBV2	779	1033	0.11%	0.012%
48	16.598	2310	2314	2316	rBV4	741	1229	0.13%	0.014%
49	17.227	2415	2421	2432	rBV	369982	516351	53.02%	5.913%
50	17.327	2432	2438	2457	rVB	474243	703629	72.25%	8.058%
51	17.598	2481	2484	2489	rVB4	958	1284	0.13%	0.015%
52	17.745	2508	2509	2514	rVV2	1213	1020	0.10%	0.012%
53	18.080	2563	2566	2573	rBV5	5506	10648	1.09%	0.122%
54	18.186	2582	2584	2588	rVB4	1196	1367	0.14%	0.016%
55	18.404	2618	2621	2624	rBV4	992	1165	0.12%	0.013%
56	18.503	2630	2638	2639	rBV3	1073	2523	0.26%	0.029%
57	18.586	2650	2652	2654	rBV2	973	1298	0.13%	0.015%
58	18.774	2682	2684	2686	rVV2	1005	1015	0.10%	0.012%
59	19.103	2735	2740	2741	rBV2	1275	1343	0.14%	0.015%
60	19.186	2751	2754	2758	rVB4	3593	4223	0.43%	0.048%
61	19.262	2761	2767	2771	rBV7	3996	6754	0.69%	0.077%
62	19.368	2783	2785	2786	rBV2	2201	1515	0.16%	0.017%
63	19.433	2792	2796	2797	rVB4	1014	1031	0.11%	0.012%
64	19.621	2822	2828	2844	rBV	689614	898517	92.26%	10.290%
65	19.809	2858	2860	2864	rBV5	1704	1570	0.16%	0.018%
66	20.203	2926	2927	2930	rBV3	2031	2546	0.26%	0.029%
67	21.409	3127	3132	3145	rBV	432394	609228	62.55%	6.977%
68	23.615	3500	3507	3523	rBV	465131	973921	100.00%	11.154%
69	23.768	3526	3533	3547	rVB	332903	710702	72.97%	8.139%




Sum of corrected areas: 8731922

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042874.D
Acq On : 18 Nov 2023 10:03
Operator : MA/JU
Sample : 05226-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCGB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

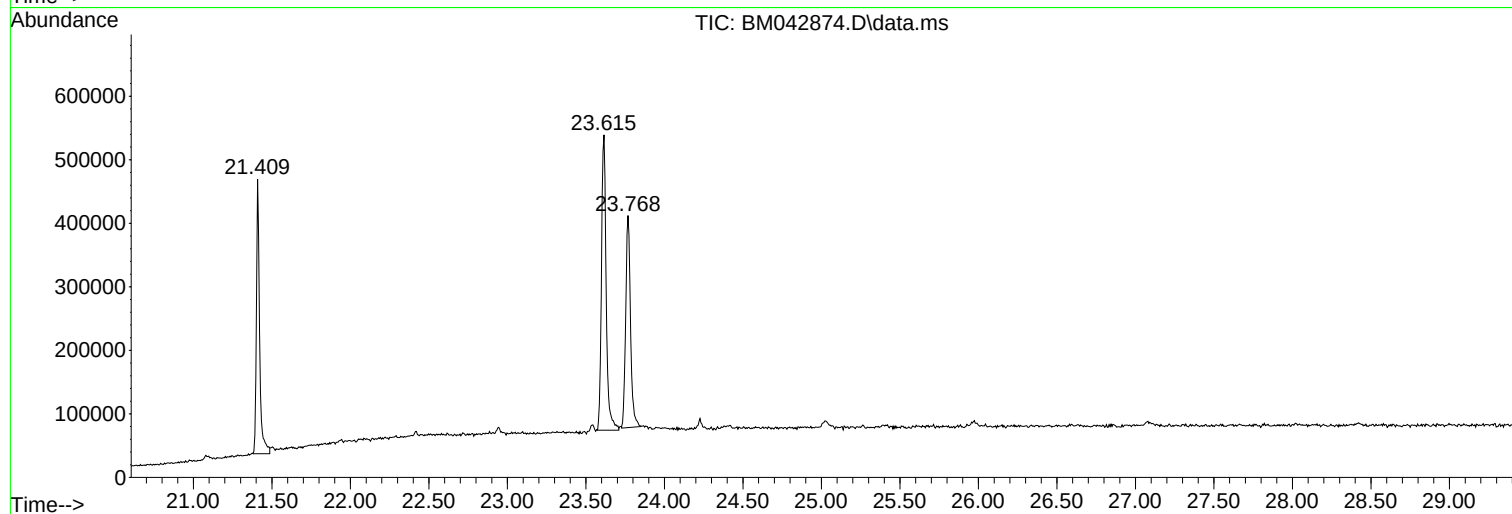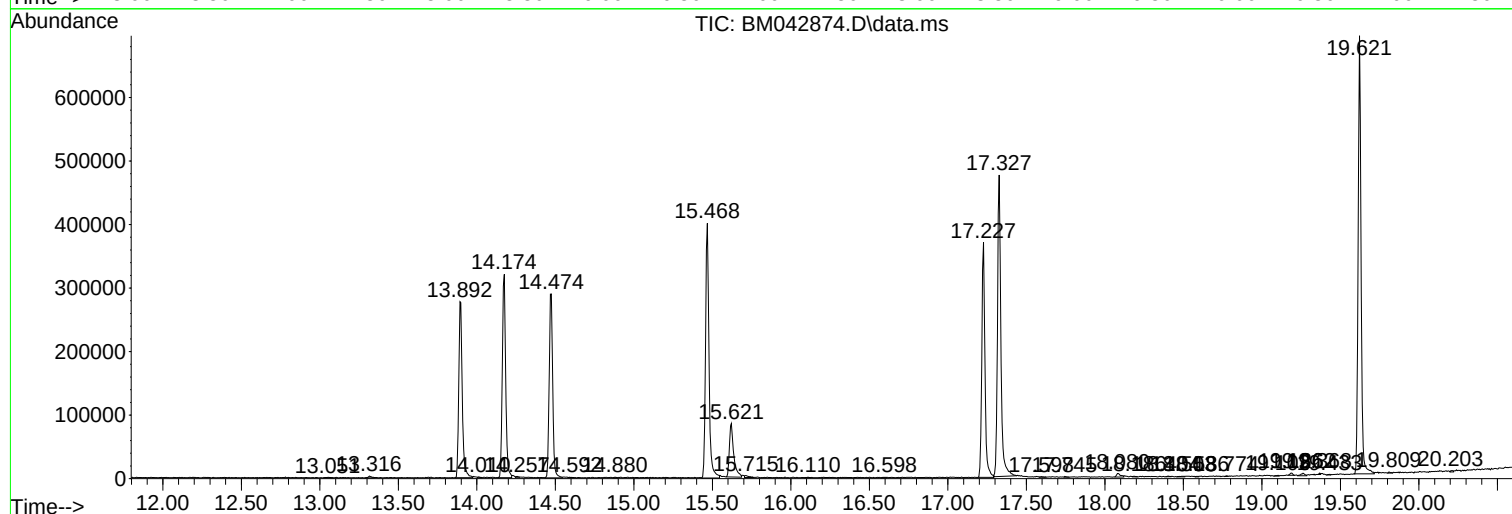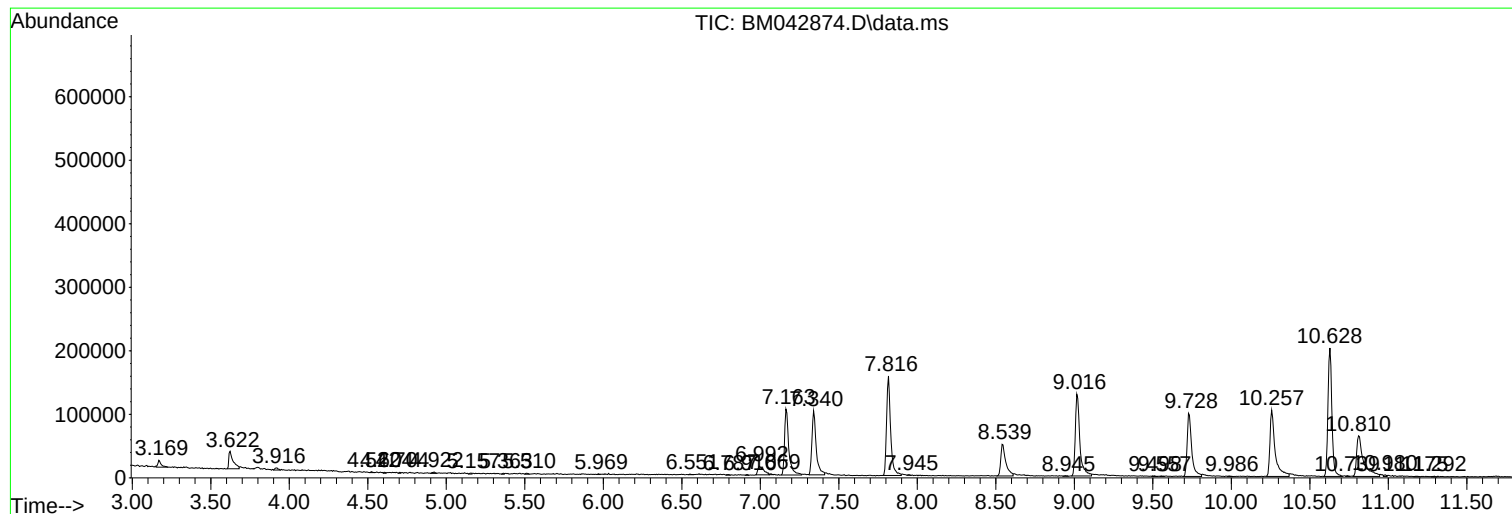

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042874.D
Acq On : 18 Nov 2023 10:03
Operator : MA/JU
Sample : 05226-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCGB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042874.D
Acq On : 18 Nov 2023 10:03
Operator : MA/JU
Sample : 05226-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCGB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------