

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042877.D
 Acq On : 18 Nov 2023 11:51
 Operator : MA/JU
 Sample : 05226-20
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	35	rBV3	7168	9224	0.90%	0.101%
2	3.622	105	108	117	rBV	25960	48909	4.80%	0.538%
3	3.916	156	158	161	rVB3	3294	2490	0.24%	0.027%
4	5.452	418	419	422	rVB2	1908	1079	0.11%	0.012%
5	6.057	520	522	526	rBV4	1243	1368	0.13%	0.015%
6	6.610	613	616	618	rBV3	2227	2078	0.20%	0.023%
7	6.775	643	644	648	rBV4	935	1091	0.11%	0.012%
8	6.863	657	659	662	rVB3	1186	1053	0.10%	0.012%
9	6.998	674	682	695	rBV3	13064	39684	3.89%	0.436%
10	7.163	705	710	725	rBV	110196	196598	19.28%	2.162%
11	7.340	733	740	750	rBV	103870	193678	18.99%	2.130%
12	7.816	815	821	835	rBV	149851	275408	27.00%	3.028%
13	7.981	847	849	852	rVB3	1154	1090	0.11%	0.012%
14	8.540	938	944	960	rBV	51148	120245	11.79%	1.322%
15	8.969	1014	1017	1018	rBV3	932	1136	0.11%	0.012%
16	9.016	1018	1025	1040	rBV	134620	267523	26.23%	2.942%
17	9.198	1053	1056	1062	rVB5	1802	3426	0.34%	0.038%
18	9.728	1140	1146	1164	rBV	109481	216759	21.25%	2.384%
19	9.892	1172	1174	1177	rVB2	909	1073	0.11%	0.012%
20	9.957	1182	1185	1190	rVB4	1258	2226	0.22%	0.024%
21	10.257	1228	1236	1255	rBV	115998	264828	25.97%	2.912%
22	10.375	1255	1256	1265	rVB6	3516	5693	0.56%	0.063%
23	10.628	1292	1299	1308	rBV	204844	346683	33.99%	3.812%
24	10.739	1316	1318	1321	rVB3	1024	1132	0.11%	0.012%
25	10.810	1324	1330	1342	rBV2	69601	179103	17.56%	1.969%
26	11.010	1362	1364	1369	rVB3	1099	1308	0.13%	0.014%
27	11.422	1432	1434	1439	rVB2	961	1253	0.12%	0.014%
28	11.633	1467	1470	1471	rBV3	1074	1100	0.11%	0.012%
29	12.257	1572	1576	1582	rVB5	1296	2298	0.23%	0.025%
30	12.786	1663	1666	1668	rVB4	1116	1069	0.10%	0.012%
31	13.045	1708	1710	1715	rVB3	1691	1752	0.17%	0.019%
32	13.322	1751	1757	1761	rVV4	2595	4343	0.43%	0.048%
33	13.692	1816	1820	1824	rVB3	1075	1464	0.14%	0.016%
34	13.892	1848	1854	1868	rBV	326641	484370	47.49%	5.326%
35	14.169	1895	1901	1909	rBV2	345851	529174	51.89%	5.819%
36	14.469	1946	1952	1963	rBV	299450	435692	42.72%	4.791%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042877.D
 Acq On : 18 Nov 2023 11:51
 Operator : MA/JU
 Sample : 05226-20
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.810	2003	2010	2011	rBV3	1386	1487	0.15%	0.016%
38	14.874	2017	2021	2025	rBV4	900	1936	0.19%	0.021%
39	15.216	2075	2079	2081	rVB4	1237	1404	0.14%	0.015%
40	15.292	2090	2092	2097	rVB3	696	1090	0.11%	0.012%
41	15.469	2116	2122	2135	rBV	450067	672540	65.94%	7.395%
42	15.557	2135	2137	2142	rVV4	2692	4320	0.42%	0.048%
43	15.616	2142	2147	2161	rVV2	104552	186124	18.25%	2.047%
44	15.751	2168	2170	2174	rVB	1331	1587	0.16%	0.017%
45	15.969	2203	2207	2210	rVB3	761	1213	0.12%	0.013%
46	16.427	2282	2285	2290	rVB5	731	1049	0.10%	0.012%
47	16.504	2290	2298	2300	rBV5	950	2198	0.22%	0.024%
48	17.227	2415	2421	2431	rBV	341634	508711	49.88%	5.594%
49	17.327	2431	2438	2455	rVV	487037	741642	72.72%	8.155%
50	17.563	2475	2478	2482	rBV	719	1117	0.11%	0.012%
51	17.833	2521	2524	2525	rBV3	1508	1728	0.17%	0.019%
52	18.080	2561	2566	2579	rBV6	12117	25705	2.52%	0.283%
53	18.162	2579	2580	2586	rVB3	1335	1997	0.20%	0.022%
54	18.433	2625	2626	2630	rBV4	1406	1249	0.12%	0.014%
55	18.509	2635	2639	2642	rVV6	1266	1864	0.18%	0.020%
56	18.533	2642	2643	2649	rVV4	1053	1410	0.14%	0.016%
57	18.715	2670	2674	2676	rVV4	793	1347	0.13%	0.015%
58	19.157	2744	2749	2750	rBV4	1317	1643	0.16%	0.018%
59	19.186	2750	2754	2757	rVV3	4261	5507	0.54%	0.061%
60	19.257	2764	2766	2770	rBV3	4734	4637	0.45%	0.051%
61	19.362	2780	2784	2793	rBV5	9918	18346	1.80%	0.202%
62	19.504	2805	2808	2810	rBV4	1688	2029	0.20%	0.022%
63	19.621	2822	2828	2840	rVV	757983	959269	94.06%	10.548%
64	19.809	2859	2860	2863	rVB3	2317	1551	0.15%	0.017%
65	20.009	2892	2894	2895	rBV2	2196	1211	0.12%	0.013%
66	21.409	3127	3132	3143	rBV	412312	580848	56.95%	6.387%
67	23.615	3500	3507	3525	rBV	503985	1019873	100.00%	11.215%
68	23.768	3526	3533	3550	rVB	324277	689987	67.65%	7.587%




Sum of corrected areas: 9094019

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042877.D
Acq On : 18 Nov 2023 11:51
Operator : MA/JU
Sample : 05226-20
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG81

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

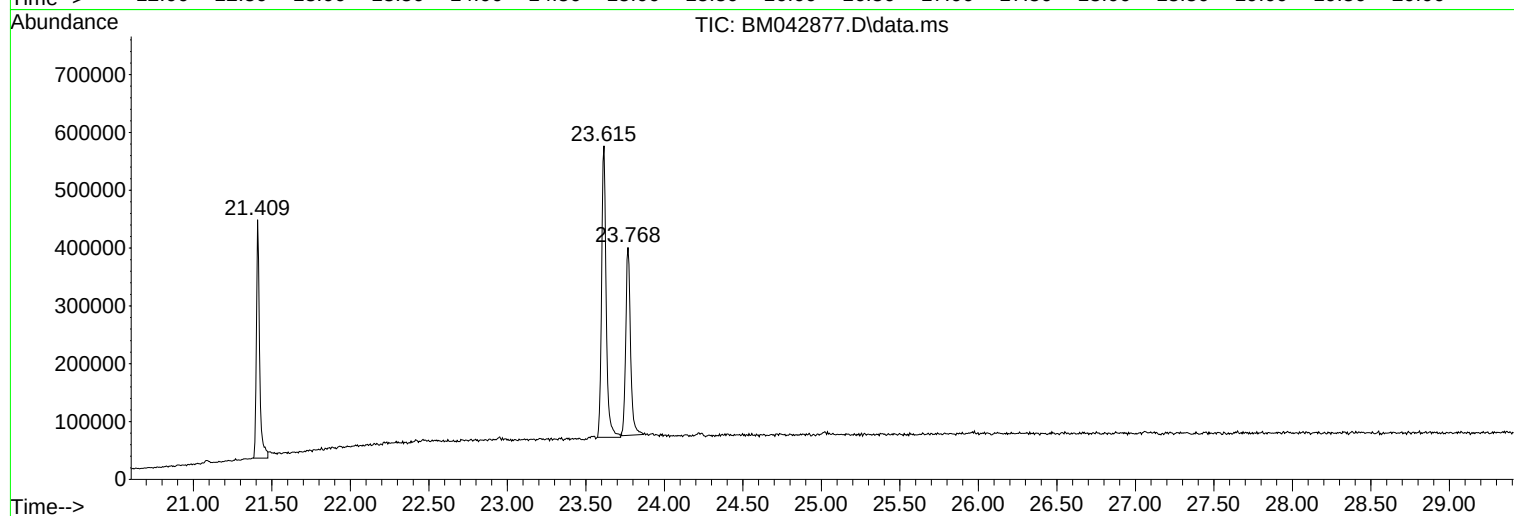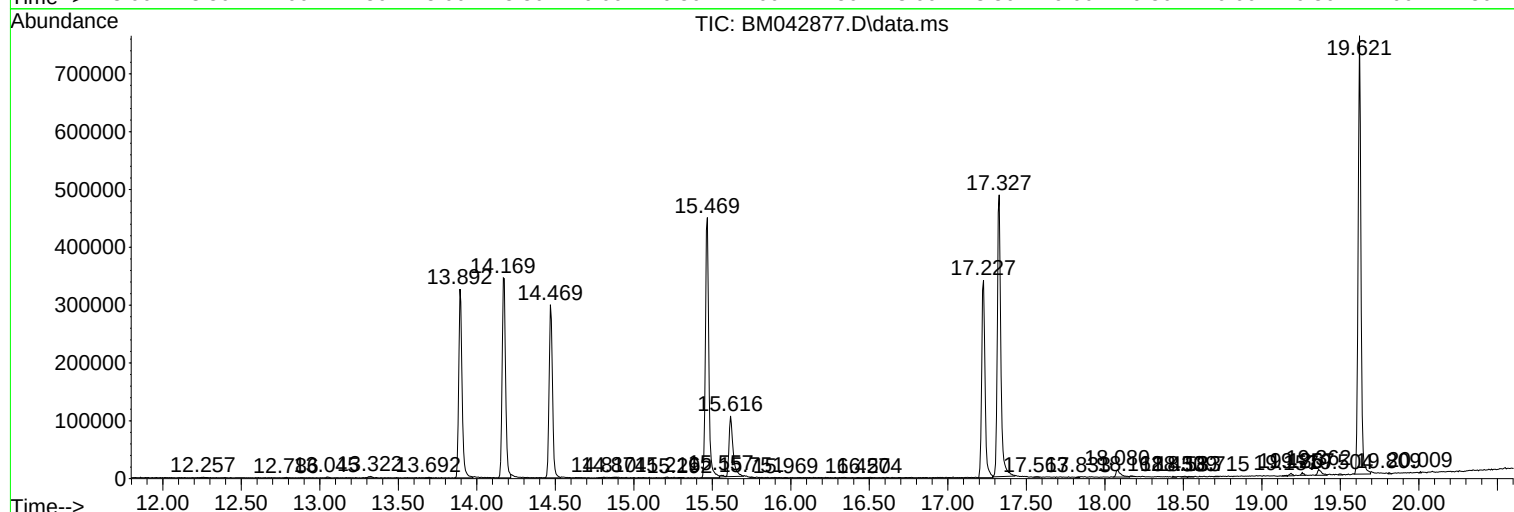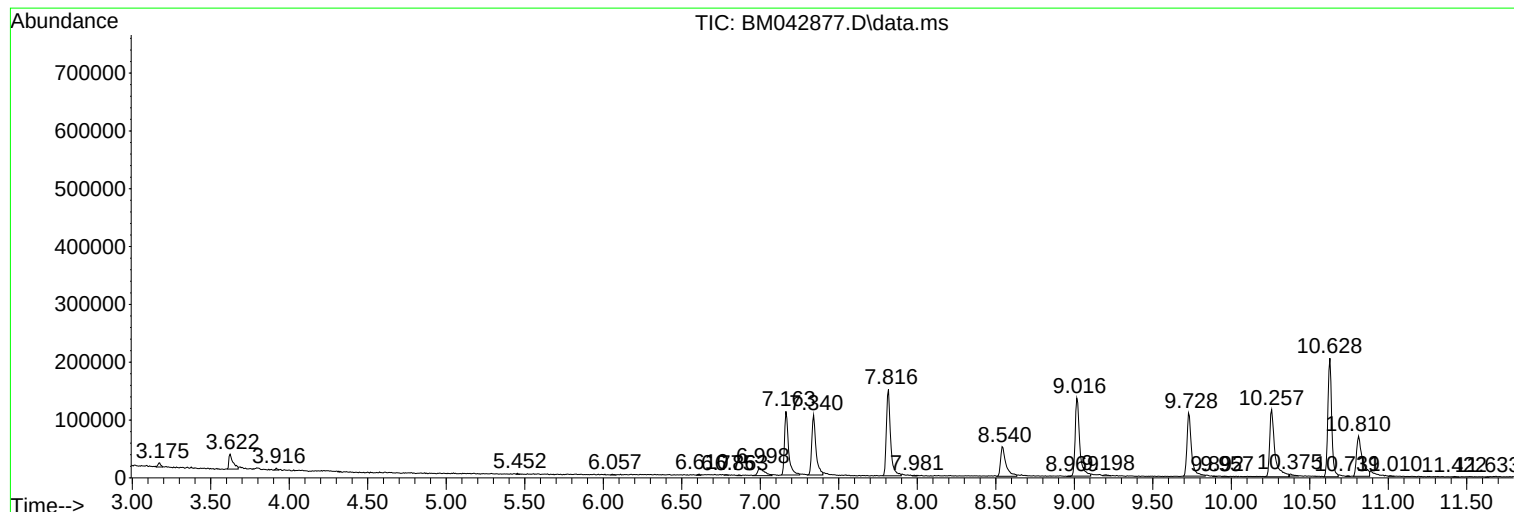

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042877.D
Acq On : 18 Nov 2023 11:51
Operator : MA/JU
Sample : 05226-20
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG81

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042877.D
Acq On : 18 Nov 2023 11:51
Operator : MA/JU
Sample : 05226-20
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG81

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------