

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042885.D
 Acq On : 18 Nov 2023 17:20
 Operator : MA/JU
 Sample : PB157269BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	34	rVB2	10705	10472	1.14%	0.125%
2	3.611	102	106	123	rBV	130830	232940	25.46%	2.789%
3	3.981	168	169	170	rBV	2860	1023	0.11%	0.012%
4	4.093	186	188	190	rBV2	2252	1663	0.18%	0.020%
5	4.799	307	308	310	rBV2	1839	1052	0.12%	0.013%
6	4.840	314	315	318	rBV3	1822	972	0.11%	0.012%
7	5.675	454	457	458	rBV3	1178	1148	0.13%	0.014%
8	5.946	501	503	504	rBV2	1207	934	0.10%	0.011%
9	6.328	565	568	570	rVB3	1489	1349	0.15%	0.016%
10	6.346	570	571	575	rBV4	999	1329	0.15%	0.016%
11	6.716	633	634	636	rVB2	1664	1025	0.11%	0.012%
12	6.793	646	647	649	rVB2	1542	976	0.11%	0.012%
13	6.981	673	679	699	rBV	138316	284960	31.15%	3.412%
14	7.163	704	710	726	rVV	116495	206689	22.59%	2.474%
15	7.263	726	727	733	rVV4	1943	2249	0.25%	0.027%
16	7.334	733	739	758	rVV	158232	292446	31.97%	3.501%
17	7.816	815	821	831	rBV	76397	149253	16.32%	1.787%
18	8.004	852	853	856	rBV	1266	1147	0.13%	0.014%
19	8.069	862	864	869	rVB3	758	1156	0.13%	0.014%
20	8.351	911	912	916	rVV2	891	1077	0.12%	0.013%
21	8.398	919	920	924	rVB3	1183	1138	0.12%	0.014%
22	8.534	937	943	965	rBV	149849	299870	32.78%	3.590%
23	8.798	987	988	995	rVB4	1250	1467	0.16%	0.018%
24	9.016	1019	1025	1043	rBV	139608	275126	30.08%	3.294%
25	9.204	1056	1057	1060	rVB3	1091	923	0.10%	0.011%
26	9.304	1071	1074	1076	rBV3	1440	1329	0.15%	0.016%
27	9.345	1078	1081	1084	rVB3	1609	1689	0.18%	0.020%
28	9.728	1140	1146	1159	rBV2	118553	228627	24.99%	2.737%
29	10.175	1220	1222	1225	rBV3	1028	1060	0.12%	0.013%
30	10.257	1228	1236	1251	rBV	130815	287985	31.48%	3.448%
31	10.628	1291	1299	1308	rBV	108265	193424	21.14%	2.316%
32	10.804	1323	1329	1350	rBV2	97836	268843	29.39%	3.219%
33	11.492	1442	1446	1448	rBV3	767	1191	0.13%	0.014%
34	11.592	1460	1463	1466	rBV4	1096	1242	0.14%	0.015%
35	11.681	1475	1478	1481	rVV4	865	1273	0.14%	0.015%
36	12.263	1574	1577	1579	rBV3	826	926	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042885.D
 Acq On : 18 Nov 2023 17:20
 Operator : MA/JU
 Sample : PB157269BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.322	1754	1757	1761	rVB2	1399	1684	0.18%	0.020%
38	13.504	1786	1788	1793	rBV4	806	987	0.11%	0.012%
39	13.827	1840	1843	1847	rBV2	948	1010	0.11%	0.012%
40	13.892	1848	1854	1869	rBV	303681	464010	50.72%	5.555%
41	14.169	1894	1901	1916	rBV	338996	516259	56.44%	6.181%
42	14.469	1946	1952	1963	rBV	157578	239503	26.18%	2.867%
43	14.569	1965	1969	1971	rVB4	1311	1553	0.17%	0.019%
44	14.627	1977	1979	1982	rBV2	806	998	0.11%	0.012%
45	14.745	1992	1999	2020	rBV5	25041	118140	12.91%	1.414%
46	14.916	2027	2028	2033	rVB5	1448	1308	0.14%	0.016%
47	14.969	2035	2037	2039	rVB3	1278	927	0.10%	0.011%
48	15.069	2051	2054	2058	rVB4	642	947	0.10%	0.011%
49	15.163	2067	2070	2072	rVB2	846	942	0.10%	0.011%
50	15.257	2083	2086	2088	rVB2	1041	1019	0.11%	0.012%
51	15.463	2115	2121	2136	rBV	420404	640438	70.01%	7.667%
52	15.574	2136	2140	2142	rVB3	1271	1405	0.15%	0.017%
53	15.616	2142	2147	2161	rBV	94363	166981	18.25%	1.999%
54	16.092	2225	2228	2231	rBV4	1106	1230	0.13%	0.015%
55	16.251	2250	2255	2258	rBV3	803	1550	0.17%	0.019%
56	16.616	2313	2317	2319	rBV	788	983	0.11%	0.012%
57	16.674	2325	2327	2331	rBV3	846	1293	0.14%	0.015%
58	17.021	2382	2386	2388	rVB3	901	1058	0.12%	0.013%
59	17.227	2415	2421	2431	rBV	178568	276383	30.21%	3.309%
60	17.327	2431	2438	2454	rVV2	418797	676230	73.92%	8.096%
61	17.615	2483	2487	2489	rBV3	736	931	0.10%	0.011%
62	17.715	2502	2504	2506	rBV3	800	947	0.10%	0.011%
63	18.074	2562	2565	2568	rBV5	944	1237	0.14%	0.015%
64	18.351	2609	2612	2614	rVV3	1169	970	0.11%	0.012%
65	18.504	2636	2638	2641	rVV4	917	1257	0.14%	0.015%
66	18.615	2656	2657	2660	rVB3	1314	970	0.11%	0.012%
67	18.651	2660	2663	2665	rBV4	1275	1530	0.17%	0.018%
68	18.915	2705	2708	2710	rVB4	937	943	0.10%	0.011%
69	19.027	2725	2727	2730	rVB4	1550	1221	0.13%	0.015%
70	19.115	2737	2742	2744	rBV4	1074	1567	0.17%	0.019%
71	19.192	2751	2755	2758	rBV5	4491	5659	0.62%	0.068%
72	19.262	2764	2767	2771	rVB3	2450	3035	0.33%	0.036%
73	19.433	2792	2796	2798	rBV4	1361	1520	0.17%	0.018%
74	19.580	2818	2821	2822	rVB2	1415	964	0.11%	0.012%
75	19.621	2822	2828	2843	rBV	615060	855798	93.55%	10.246%
76	19.986	2888	2890	2891	rBV2	1661	1649	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042885.D
Acq On : 18 Nov 2023 17:20
Operator : MA/JU
Sample : PB157269BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK269

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	20.592	2991	2993	2994	rBV	3486	2435	0.27%	0.029%
78	21.415	3128	3133	3145	rBV	184764	309326	33.81%	3.703%
79	23.615	3500	3507	3524	rBV2	440721	914782	100.00%	10.952%
80	23.774	3527	3534	3548	rVB	160458	369235	40.36%	4.421%




Sum of corrected areas: 8352787

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042885.D
Acq On : 18 Nov 2023 17:20
Operator : MA/JU
Sample : PB157269BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK269

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

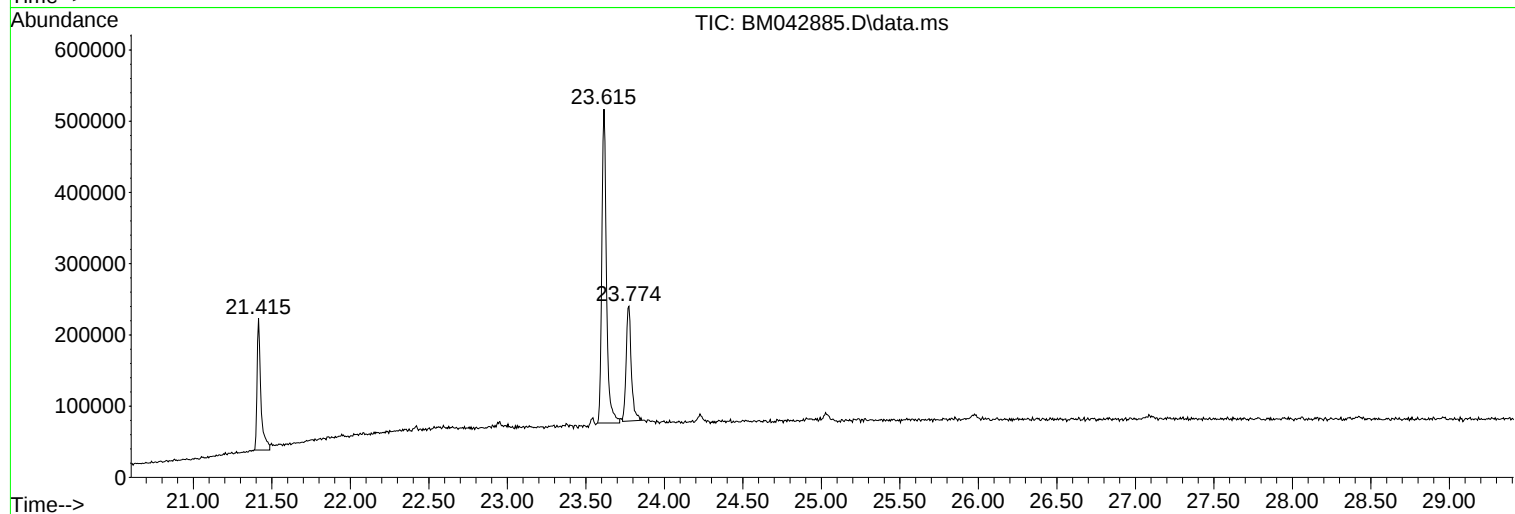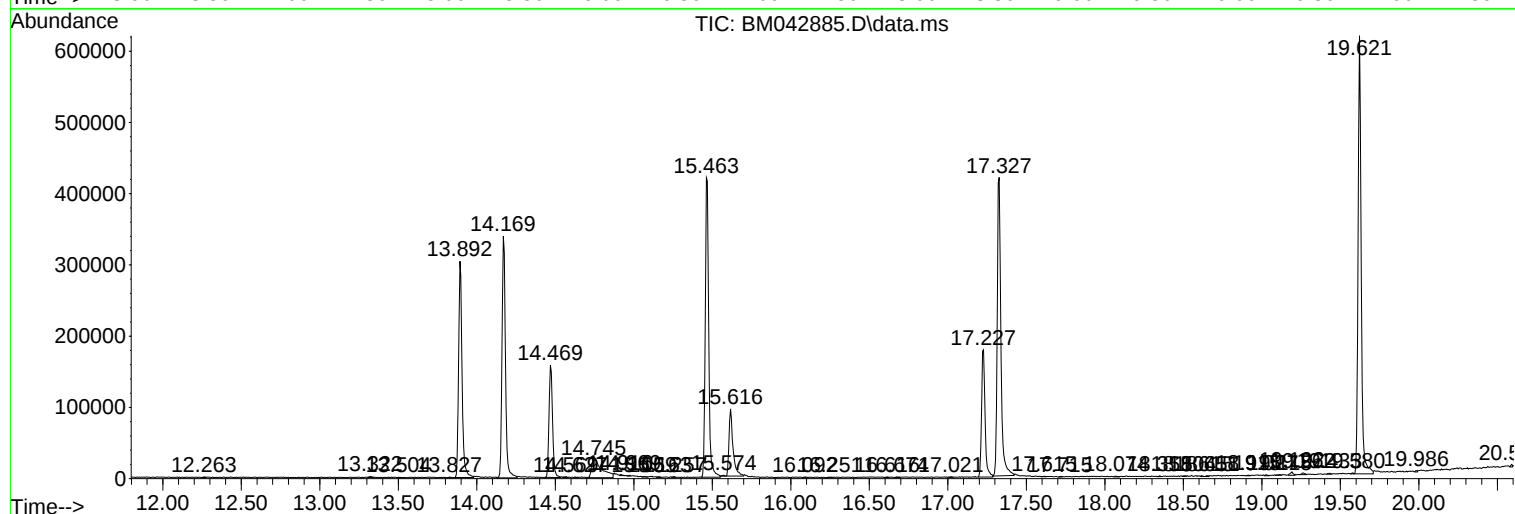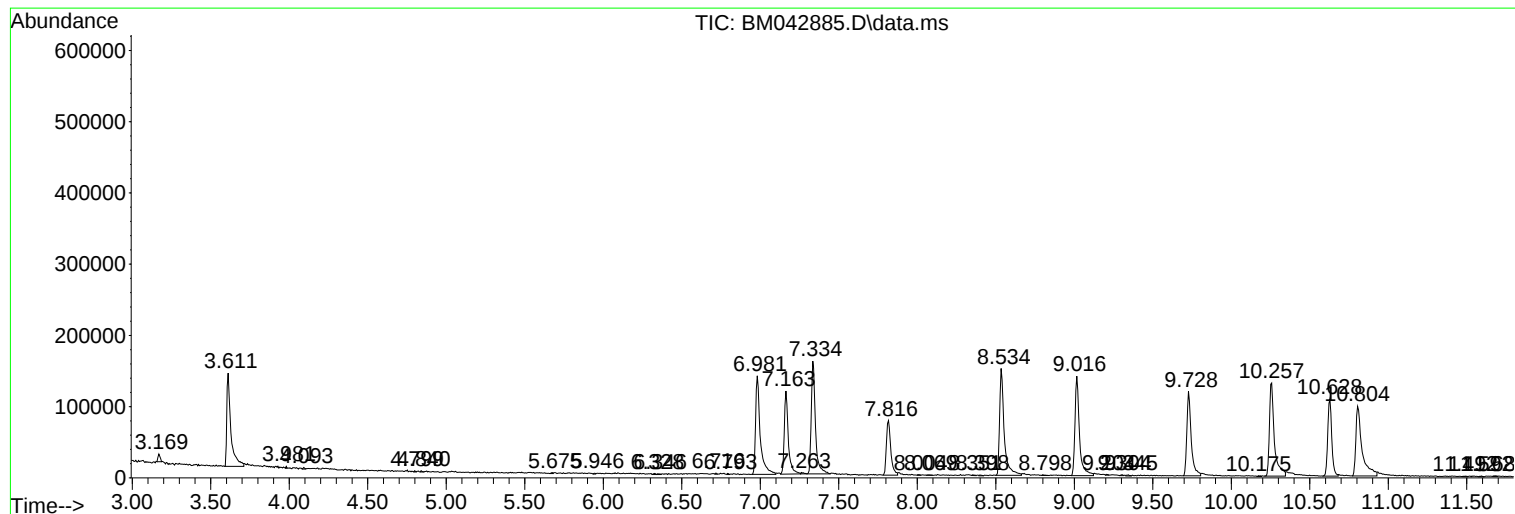

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042885.D
Acq On : 18 Nov 2023 17:20
Operator : MA/JU
Sample : PB157269BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK269

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042885.D
Acq On : 18 Nov 2023 17:20
Operator : MA/JU
Sample : PB157269BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK269

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------