

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042886.D
 Acq On : 18 Nov 2023 17:56
 Operator : MA/JU
 Sample : 05370-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCDQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	41	rVB5	9109	12135	1.30%	0.167%
2	3.622	105	108	122	rBV	27525	52746	5.67%	0.724%
3	3.916	156	158	162	rBV5	2603	4022	0.43%	0.055%
4	4.446	246	248	251	rBV3	1154	1206	0.13%	0.017%
5	4.869	318	320	323	rBV3	1180	1045	0.11%	0.014%
6	4.899	323	325	326	rVB2	2134	1342	0.14%	0.018%
7	4.916	326	328	332	rBV4	1991	3259	0.35%	0.045%
8	5.775	472	474	476	rBV3	1002	1031	0.11%	0.014%
9	6.193	543	545	548	rVB3	1312	995	0.11%	0.014%
10	6.610	614	616	617	rBV2	1201	965	0.10%	0.013%
11	6.687	627	629	631	rBV3	1870	1807	0.19%	0.025%
12	6.769	640	643	645	rBV3	1261	1454	0.16%	0.020%
13	6.816	648	651	653	rBV4	1007	1039	0.11%	0.014%
14	6.993	676	681	692	rBV3	12797	36259	3.90%	0.498%
15	7.163	704	710	734	rBV	96795	188582	20.26%	2.588%
16	7.340	734	740	754	rBV	101542	194909	20.94%	2.675%
17	7.816	815	821	837	rVV	86184	163391	17.56%	2.242%
18	8.140	872	876	879	rBV5	1117	1642	0.18%	0.023%
19	8.169	879	881	884	rVV4	919	953	0.10%	0.013%
20	8.310	904	905	909	rVB3	1089	1318	0.14%	0.018%
21	8.345	909	911	915	rBV4	816	1198	0.13%	0.016%
22	8.540	939	944	957	rVV	51128	110993	11.93%	1.523%
23	8.692	968	970	972	rVB3	1465	1173	0.13%	0.016%
24	9.016	1019	1025	1041	rBV	118921	243705	26.19%	3.345%
25	9.198	1054	1056	1059	rVB3	2386	2244	0.24%	0.031%
26	9.728	1140	1146	1160	rBV	99206	194478	20.90%	2.669%
27	9.828	1162	1163	1167	rVV4	2009	2356	0.25%	0.032%
28	10.257	1230	1236	1254	rBV2	100751	232129	24.94%	3.186%
29	10.628	1292	1299	1312	rBV	123183	215929	23.20%	2.963%
30	10.733	1316	1317	1323	rVB3	737	995	0.11%	0.014%
31	10.810	1323	1330	1348	rBV	73751	206953	22.24%	2.840%
32	11.057	1370	1372	1374	rVB2	1227	965	0.10%	0.013%
33	11.081	1374	1376	1379	rVB4	1226	932	0.10%	0.013%
34	11.610	1464	1466	1470	rBV4	882	1193	0.13%	0.016%
35	12.886	1677	1683	1685	rBV2	717	1061	0.11%	0.015%
36	13.133	1720	1725	1729	rVB3	702	1264	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042886.D
 Acq On : 18 Nov 2023 17:56
 Operator : MA/JU
 Sample : 05370-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCDQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.322	1753	1757	1761	rVB2	3647	5317	0.57%	0.073%
38	13.551	1793	1796	1800	rVB3	688	1104	0.12%	0.015%
39	13.686	1817	1819	1822	rBV4	993	940	0.10%	0.013%
40	13.892	1849	1854	1867	rBV	277778	413535	44.43%	5.675%
41	14.169	1896	1901	1920	rBV	305210	465199	49.99%	6.384%
42	14.469	1945	1952	1964	rBV	171991	260492	27.99%	3.575%
43	15.110	2060	2061	2065	rVB3	918	945	0.10%	0.013%
44	15.204	2074	2077	2082	rVV3	799	1089	0.12%	0.015%
45	15.468	2116	2122	2133	rBV	366274	580497	62.37%	7.967%
46	15.616	2143	2147	2161	rVV2	77092	153233	16.46%	2.103%
47	15.710	2161	2163	2169	rVV4	3455	4398	0.47%	0.060%
48	16.492	2291	2296	2298	rBV2	795	1025	0.11%	0.014%
49	17.074	2393	2395	2397	rBV2	1076	1133	0.12%	0.016%
50	17.227	2415	2421	2432	rBV	195196	296123	31.82%	4.064%
51	17.327	2432	2438	2452	rBV	418857	650391	69.88%	8.926%
52	17.833	2521	2524	2526	rVB4	911	1089	0.12%	0.015%
53	17.851	2526	2527	2532	rBV4	1645	1965	0.21%	0.027%
54	18.098	2563	2569	2570	rBV5	2199	3680	0.40%	0.051%
55	18.298	2597	2603	2611	rBV2	10510	13979	1.50%	0.192%
56	18.539	2642	2644	2648	rVB3	1008	1415	0.15%	0.019%
57	19.086	2734	2737	2740	rBV4	762	961	0.10%	0.013%
58	19.186	2751	2754	2757	rBV3	3212	3237	0.35%	0.044%
59	19.256	2763	2766	2773	rBV3	3136	5069	0.54%	0.070%
60	19.380	2785	2787	2790	rBV4	1345	1359	0.15%	0.019%
61	19.498	2805	2807	2810	rVB3	2122	1757	0.19%	0.024%
62	19.621	2823	2828	2840	rBV	627455	850418	91.38%	11.671%
63	19.815	2860	2861	2865	rVB4	1768	1934	0.21%	0.027%
64	20.098	2908	2909	2911	rBV2	2117	1361	0.15%	0.019%
65	20.156	2917	2919	2920	rBV2	2033	1384	0.15%	0.019%
66	21.415	3128	3133	3146	rBV	209232	345995	37.18%	4.748%
67	23.615	3500	3507	3523	rBV	453632	930669	100.00%	12.773%
68	23.768	3527	3533	3545	rVB	182439	397117	42.67%	5.450%




Sum of corrected areas: 7286478

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042886.D
Acq On : 18 Nov 2023 17:56
Operator : MA/JU
Sample : 05370-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCDQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

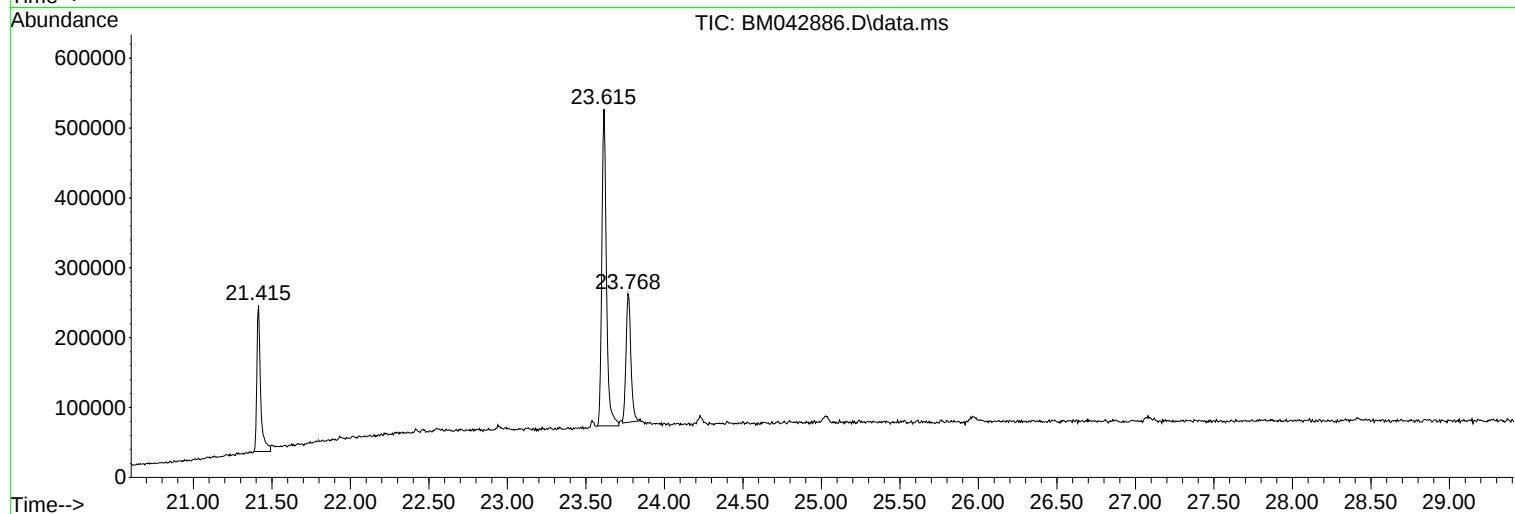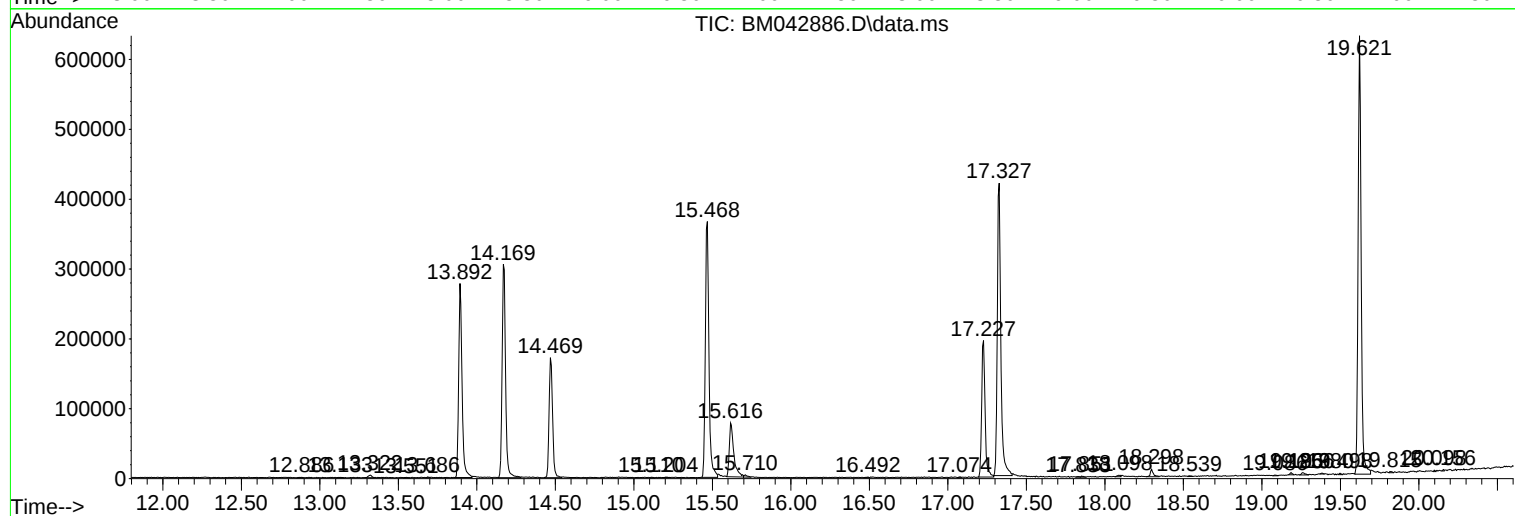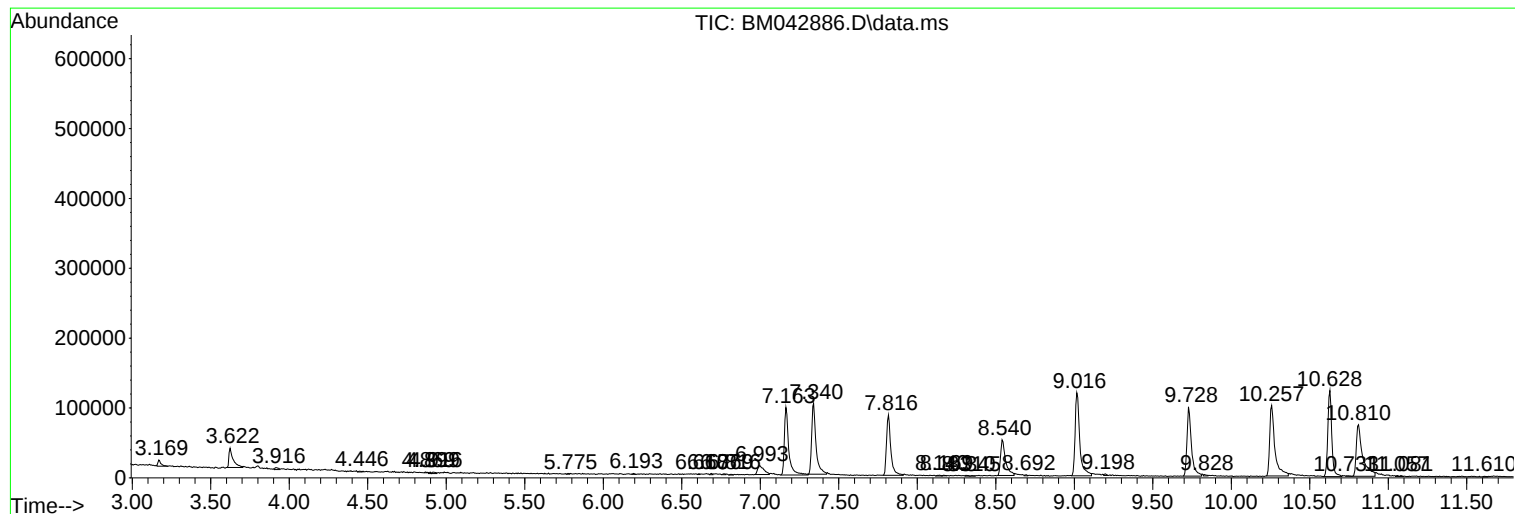

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042886.D
Acq On : 18 Nov 2023 17:56
Operator : MA/JU
Sample : 05370-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCDQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042886.D
Acq On : 18 Nov 2023 17:56
Operator : MA/JU
Sample : 05370-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCDQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------