

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042901.D
 Acq On : 19 Nov 2023 12:00
 Operator : MA/JU
 Sample : PB157215BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	37	rVB2	11813	15713	1.73%	0.167%
2	3.604	102	105	122	rBV	144688	251686	27.71%	2.671%
3	4.234	210	212	215	rBV3	1978	1345	0.15%	0.014%
4	4.487	253	255	257	rBV2	1703	1383	0.15%	0.015%
5	4.604	273	275	279	rBV3	1327	1595	0.18%	0.017%
6	4.828	310	313	314	rBV3	1153	934	0.10%	0.010%
7	4.934	329	331	334	rVB2	1536	1231	0.14%	0.013%
8	5.210	376	378	381	rVB2	1750	1384	0.15%	0.015%
9	5.534	432	433	436	rBV2	1381	1259	0.14%	0.013%
10	5.892	492	494	500	rBV4	1245	2192	0.24%	0.023%
11	6.275	556	559	561	rBV4	1326	1547	0.17%	0.016%
12	6.410	580	582	583	rBV2	1528	977	0.11%	0.010%
13	6.504	597	598	601	rVB2	1431	1414	0.16%	0.015%
14	6.545	601	605	606	rBV3	1657	1930	0.21%	0.020%
15	6.981	673	679	693	rBV	148750	297643	32.77%	3.158%
16	7.163	704	710	723	rBV	129598	224810	24.75%	2.385%
17	7.334	733	739	750	rBV	181403	309659	34.09%	3.286%
18	7.810	814	820	835	rBV	132959	242326	26.68%	2.571%
19	8.204	884	887	890	rBV4	797	925	0.10%	0.010%
20	8.451	927	929	931	rBV2	1016	1086	0.12%	0.012%
21	8.533	937	943	962	rBV	169851	325286	35.81%	3.452%
22	8.945	1011	1013	1016	rVB3	1095	1229	0.14%	0.013%
23	9.016	1018	1025	1043	rBV	148722	299475	32.97%	3.178%
24	9.192	1054	1055	1058	rVB2	1301	953	0.10%	0.010%
25	9.222	1058	1060	1066	rVB5	1043	1693	0.19%	0.018%
26	9.369	1081	1085	1086	rVV3	1070	1079	0.12%	0.011%
27	9.727	1138	1146	1156	rBV	127123	246092	27.10%	2.611%
28	10.075	1202	1205	1208	rBV2	1069	1018	0.11%	0.011%
29	10.251	1230	1235	1251	rBV	151418	319046	35.13%	3.385%
30	10.357	1251	1253	1264	rVV10	5583	15108	1.66%	0.160%
31	10.427	1264	1265	1269	rVV3	2134	2082	0.23%	0.022%
32	10.457	1269	1270	1275	rVB4	943	1006	0.11%	0.011%
33	10.622	1292	1298	1308	rBV	179632	307058	33.81%	3.258%
34	10.804	1323	1329	1340	rBV	112863	272370	29.99%	2.890%
35	10.963	1354	1356	1360	rVB5	2830	3217	0.35%	0.034%
36	10.992	1360	1361	1364	rVV3	1424	1042	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
 Data File : BM042901.D
 Acq On : 19 Nov 2023 12:00
 Operator : MA/JU
 Sample : PB157215BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	11.057	1371	1372	1378	rVB4	1080	1512	0.17%	0.016%
38	11.116	1381	1382	1385	rBV2	1094	943	0.10%	0.010%
39	11.769	1489	1493	1496	rVB2	723	967	0.11%	0.010%
40	12.033	1534	1538	1541	rVB4	736	958	0.11%	0.010%
41	12.269	1575	1578	1581	rVB2	1168	1102	0.12%	0.012%
42	12.604	1631	1635	1638	rBV2	650	1129	0.12%	0.012%
43	13.021	1703	1706	1709	rBV4	730	1035	0.11%	0.011%
44	13.315	1750	1756	1762	rBV4	2966	5978	0.66%	0.063%
45	13.380	1765	1767	1772	rVB3	858	919	0.10%	0.010%
46	13.592	1798	1803	1804	rBV3	662	1021	0.11%	0.011%
47	13.698	1818	1821	1823	rVB2	929	1007	0.11%	0.011%
48	13.892	1848	1854	1865	rBV	324031	480610	52.92%	5.100%
49	14.168	1895	1901	1916	rBV	362544	539104	59.36%	5.720%
50	14.286	1919	1921	1925	rVB3	957	992	0.11%	0.011%
51	14.404	1936	1941	1944	rVB5	871	1404	0.15%	0.015%
52	14.468	1946	1952	1962	rVV	264984	380207	41.86%	4.034%
53	14.551	1965	1966	1975	rVV3	1382	2667	0.29%	0.028%
54	14.751	1993	2000	2013	rBV3	27261	104678	11.53%	1.111%
55	14.980	2038	2039	2043	rVB3	1083	959	0.11%	0.010%
56	15.168	2069	2071	2075	rVB3	1033	1467	0.16%	0.016%
57	15.462	2115	2121	2137	rBV	449259	668359	73.59%	7.092%
58	15.615	2142	2147	2160	rBV	101853	173846	19.14%	1.845%
59	15.827	2180	2183	2186	rBV3	643	923	0.10%	0.010%
60	16.798	2344	2348	2353	rBV4	772	1329	0.15%	0.014%
61	17.015	2383	2385	2390	rBV3	828	1362	0.15%	0.014%
62	17.174	2407	2412	2413	rBV3	851	929	0.10%	0.010%
63	17.221	2415	2420	2431	rBV	285894	421738	46.43%	4.475%
64	17.321	2431	2437	2457	rVB	437879	684980	75.42%	7.268%
65	18.080	2565	2566	2569	rVB2	1173	993	0.11%	0.011%
66	18.309	2604	2605	2610	rBV4	988	1327	0.15%	0.014%
67	18.380	2614	2617	2621	rBV4	1082	1964	0.22%	0.021%
68	18.509	2636	2639	2641	rBV3	1037	1119	0.12%	0.012%
69	18.550	2643	2646	2648	rBV3	1103	1240	0.14%	0.013%
70	18.921	2706	2709	2712	rBV4	864	1124	0.12%	0.012%
71	19.109	2739	2741	2744	rBV3	1161	1632	0.18%	0.017%
72	19.150	2746	2748	2751	rVV2	998	1183	0.13%	0.013%
73	19.186	2751	2754	2760	rVB6	4052	5529	0.61%	0.059%
74	19.233	2760	2762	2763	rBV2	954	923	0.10%	0.010%
75	19.262	2763	2767	2770	rBV2	2544	3561	0.39%	0.038%
76	19.321	2775	2777	2782	rVV5	1670	2332	0.26%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042901.D
Acq On : 19 Nov 2023 12:00
Operator : MA/JU
Sample : PB157215BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	19.374	2785	2786	2790	rBV3	966	1059	0.12%	0.011%
78	19.621	2822	2828	2843	rBV	608833	838679	92.34%	8.899%
79	19.786	2854	2856	2857	rBV2	1568	917	0.10%	0.010%
80	19.850	2866	2867	2870	rVB3	1874	952	0.10%	0.010%
81	19.956	2883	2885	2886	rBV2	2034	1178	0.13%	0.012%
82	21.409	3127	3132	3144	rBV	304356	478185	52.65%	5.074%
83	23.609	3499	3506	3519	rBV	449310	908253	100.00%	9.638%
84	23.762	3526	3532	3545	rVB	263317	531083	58.47%	5.635%




Sum of corrected areas: 9424151

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042901.D
Acq On : 19 Nov 2023 12:00
Operator : MA/JU
Sample : PB157215BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

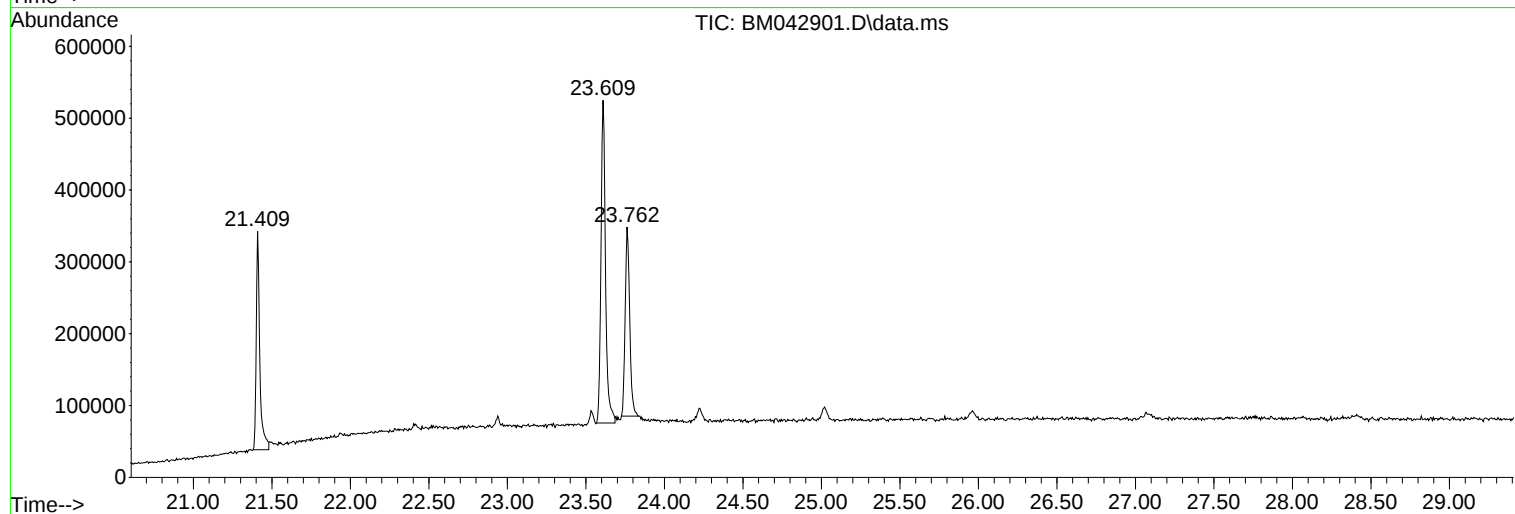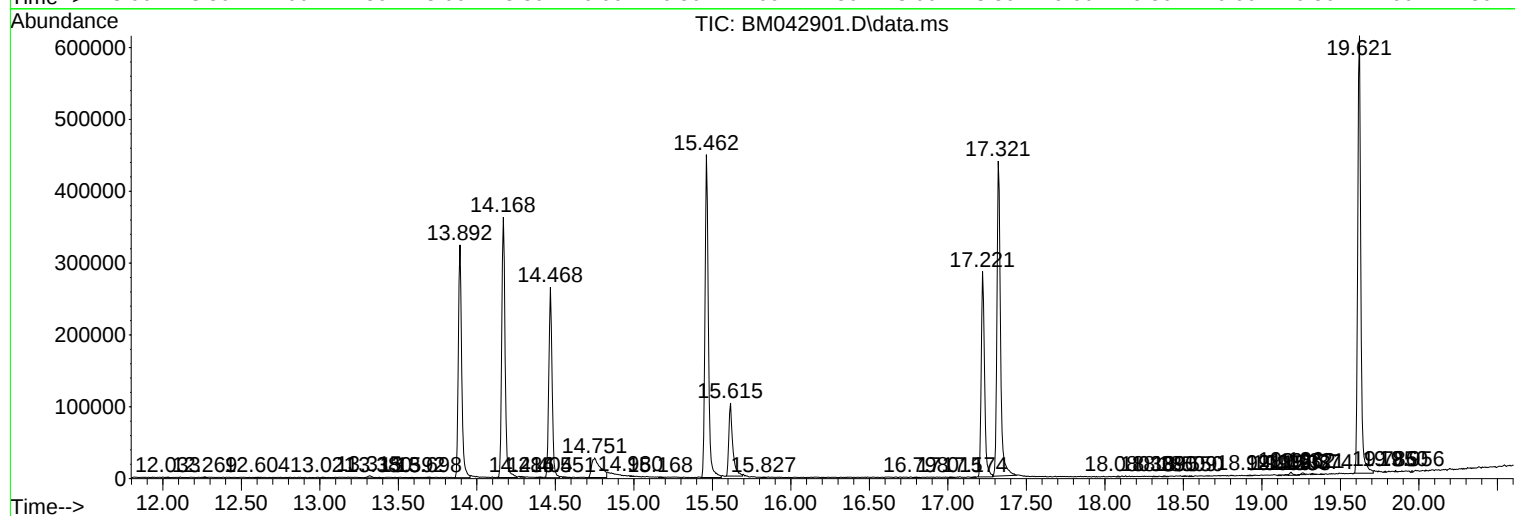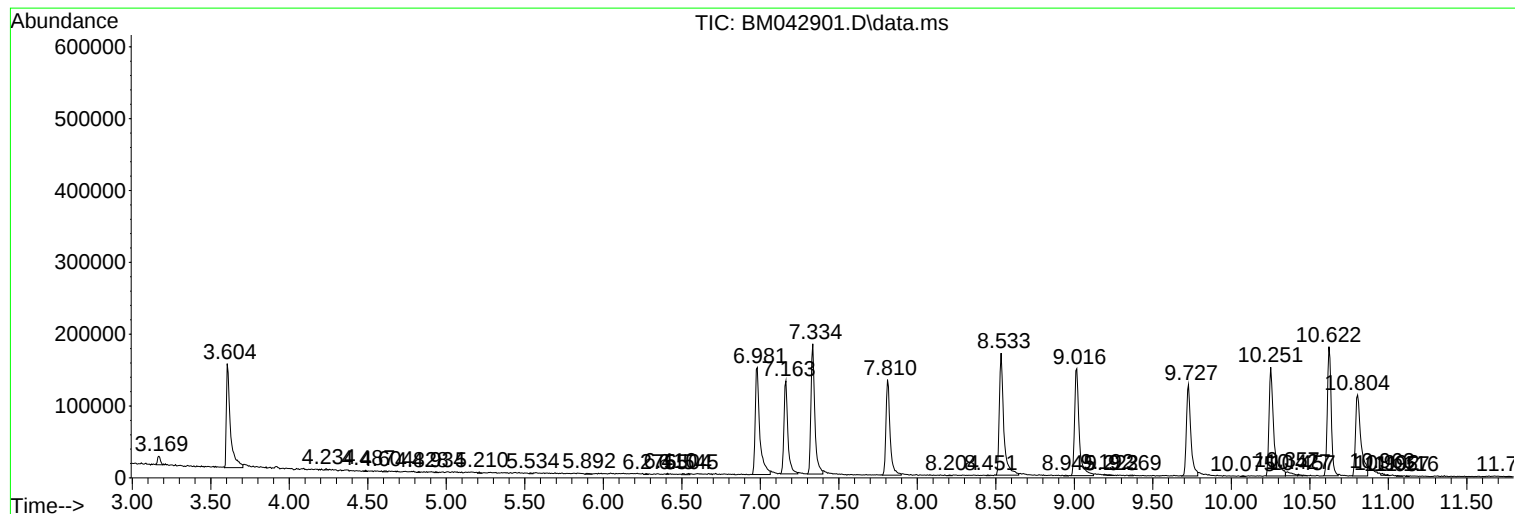

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042901.D
Acq On : 19 Nov 2023 12:00
Operator : MA/JU
Sample : PB157215BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111723\
Data File : BM042901.D
Acq On : 19 Nov 2023 12:00
Operator : MA/JU
Sample : PB157215BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------