

Data File : BM023788.D

Acq On : 18 Nov 2019 18:44

Operator : JU

Sample : SSTDCCC020EC

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Nov 19 01:07:36 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Nov 19 01:04:44 2019

Response via : Initial Calibration

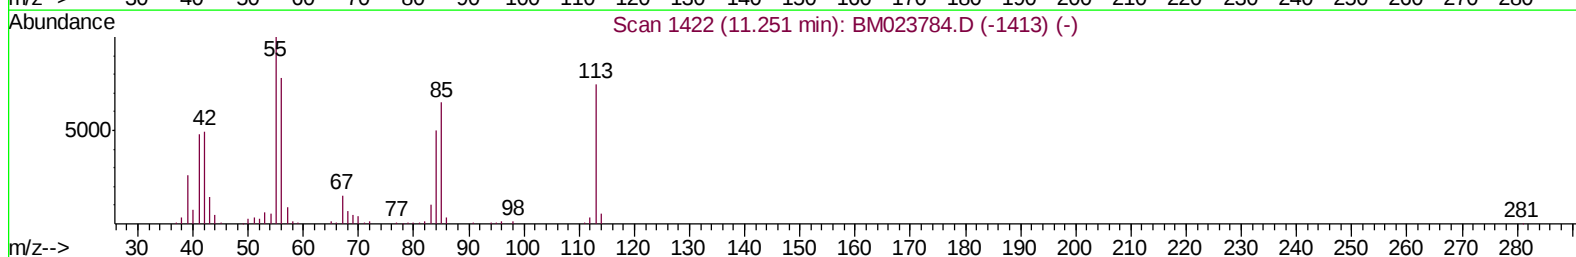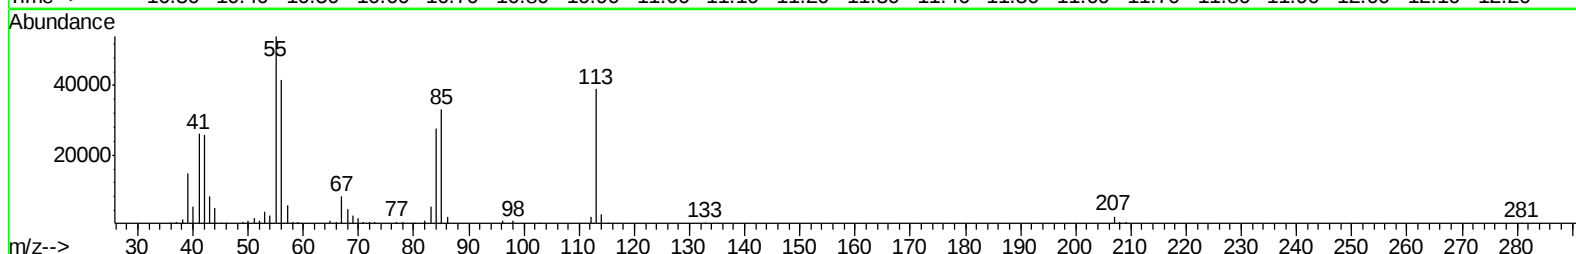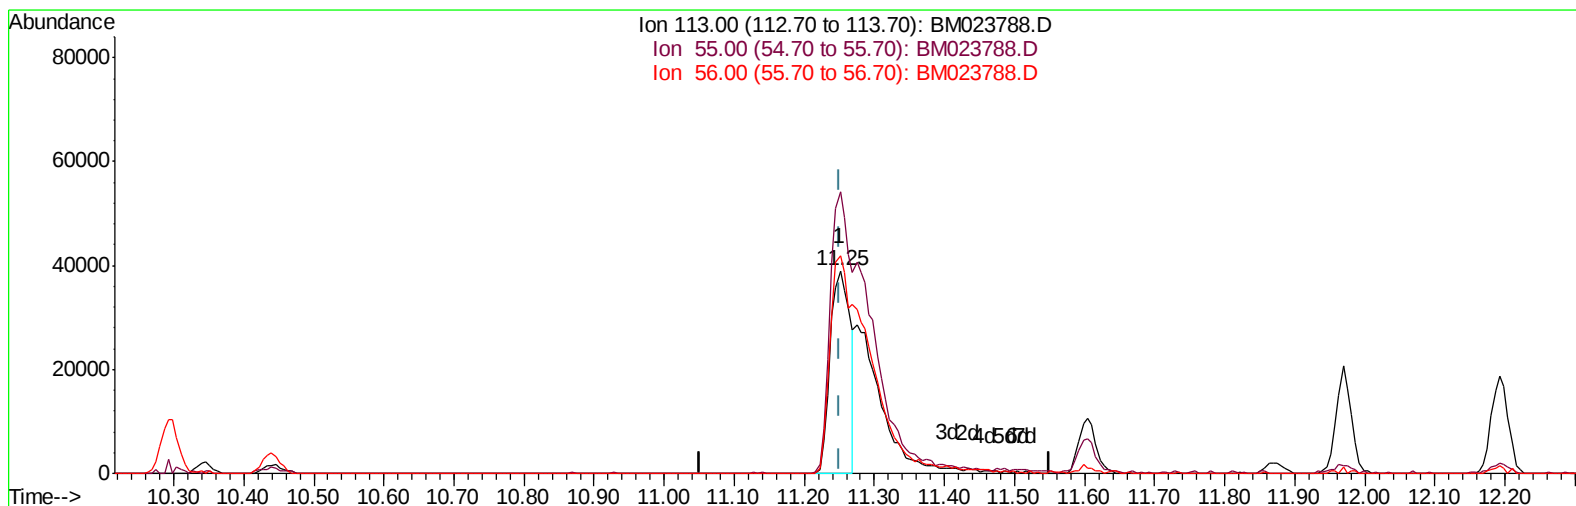

TIC: BM023788.D

(32) Caprolactam

11.251min (+0.000) 8.59ng/ul

response 78288

Ion	Exp%	Act%
113.00	100	100
55.00	132.20	138.92
56.00	103.80	107.16
0.00	0.00	0.00