

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111819\
 Data File : BM023783.D
 Acq On : 18 Nov 2019 15:42
 Operator : JU
 Sample : K5699-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F2J17

Quant Time: Nov 18 16:46:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 16 03:18:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	303127	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	1233550	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	763290	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	1609929	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1590385	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	1916422	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	35490	4.83	ng/uL	0.00
5) Phenol-d5	6.71	99	190307	6.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	475443	29.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	515211	25.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.24	113	349246	15.84	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	306731	34.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	338005	36.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.93	165	602775	28.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.45	131	53355	2.30	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	2151128	36.14	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	2396005	35.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.41	143	48048	4.73	ng/ul	0.00
58) Fluorene-d10	15.18	176	1867774	35.53	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	282866	30.37	ng/ul	0.00
71) Anthracene-d10	17.03	188	2927765	38.34	ng/ul	0.00
79) Pyrene-d10	19.33	212	3240378	39.08	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	3889266	38.57	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.64	163	155781	2.671	ng/ul	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111819\
Data File : BM023783.D
Acq On : 18 Nov 2019 15:42
Operator : JU
Sample : K5699-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F2J17

Quant Time: Nov 18 16:46:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 16 03:18:12 2019
Response via : Initial Calibration

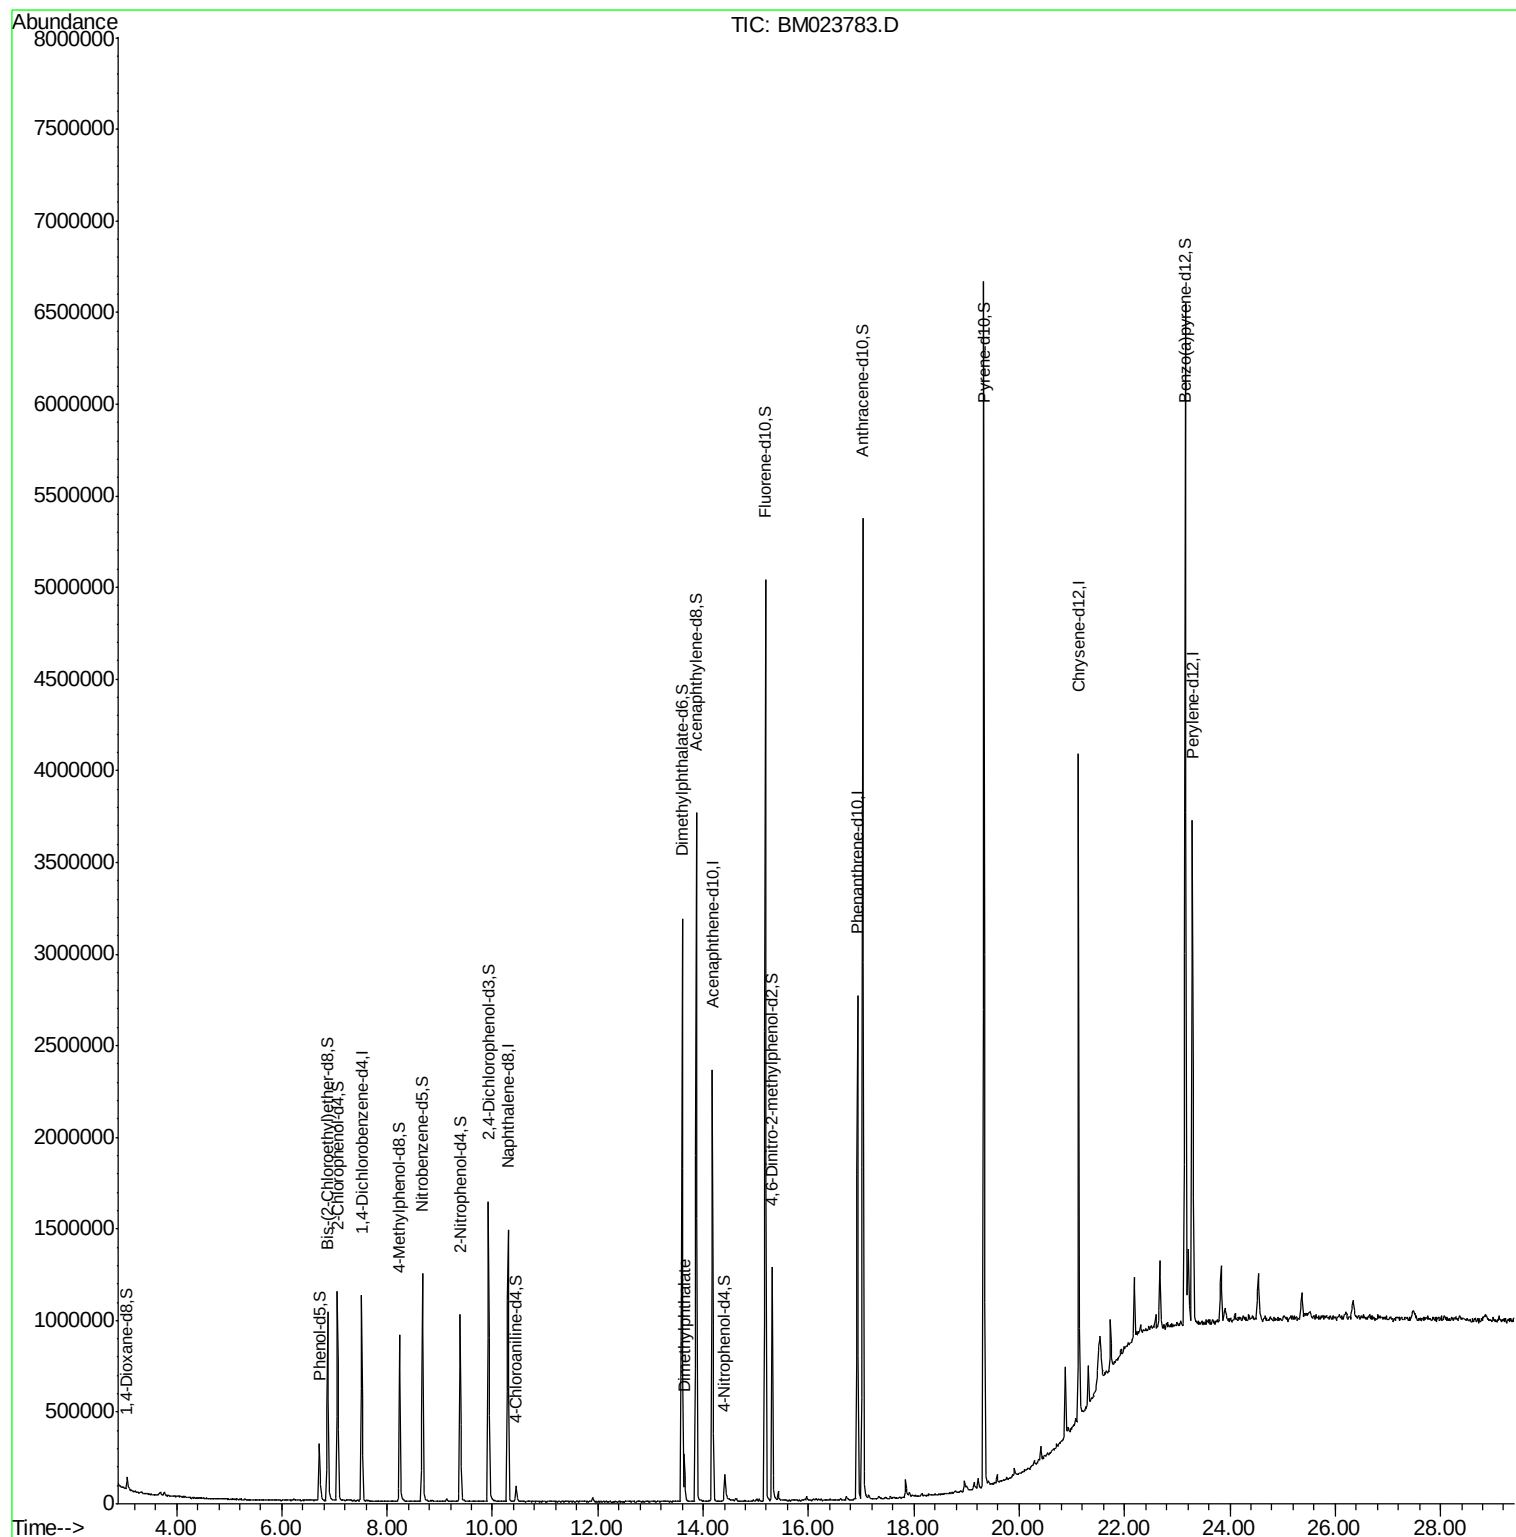

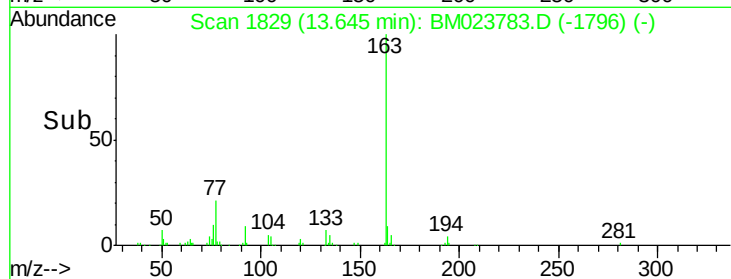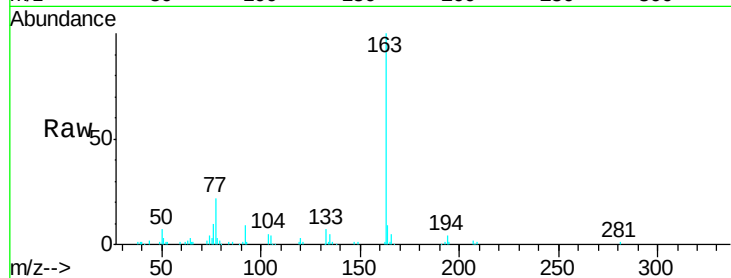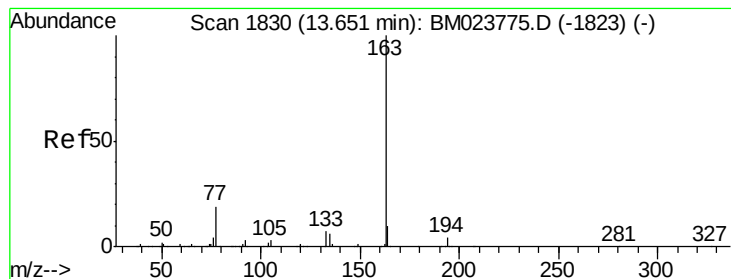

#45

Dimethylphthalate

Concen: 2.671 ng/ul

RT: 13.64 min Scan# 1829

Delta R.T. -0.01 min

Lab File: BM023783.D

Acq: 18 Nov 2019 15:42

Instrument :

BNA_M

ClientSampleId :

F2J17

Tgt Ion:163 Resp: 155781

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 9.3 8.0 12.0

