
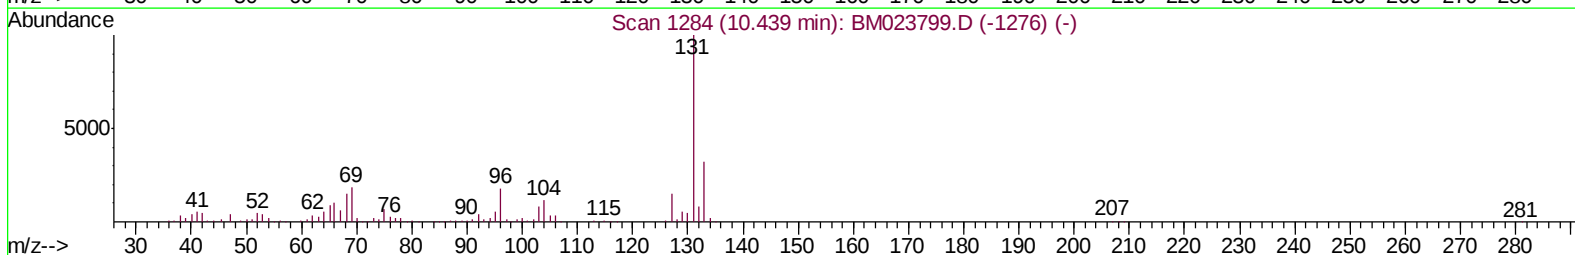
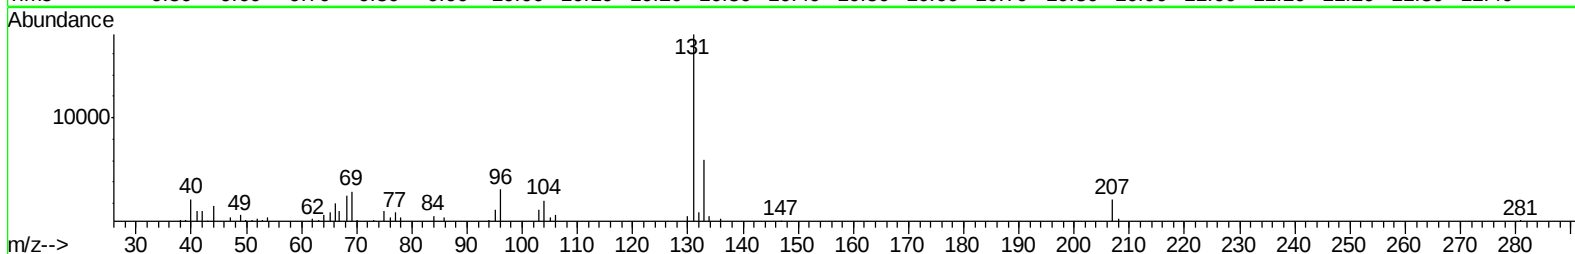


Data File : BM023802.D
Acq On : 19 Nov 2019 18:15
Operator : JU
Sample : K5748-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 20 06:57:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

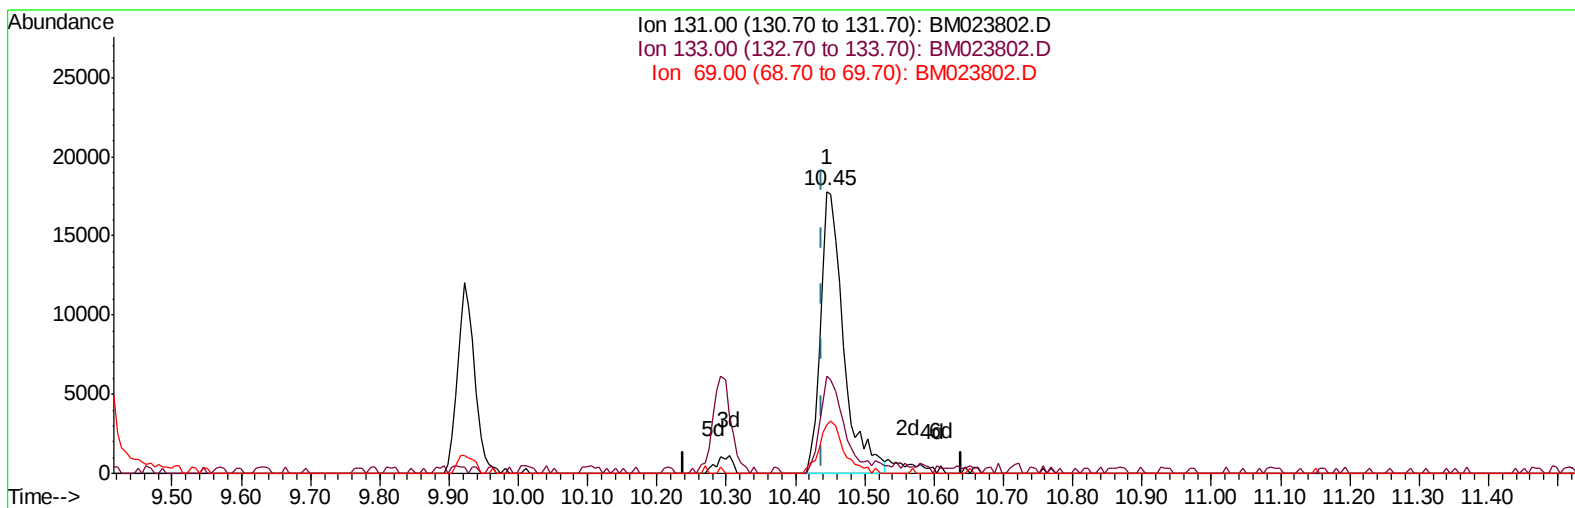

TIC: BM023802.D

(29) 4-Chloroaniline-d4 (S)

10.445min (+0.006) 1.48ng/ul m

response 40980

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	34.42
69.00	19.60	17.26
0.00	0.00	0.00