

Data File : BM023801.D
Acq On : 19 Nov 2019 17:38
Operator : JU
Sample : K5748-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEHP5

Quant Time: Nov 20 06:57:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	347849	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	1424784	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.17	164	862835	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	1841563	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1918155	20.00	ng/ul	0.00
86) Perylene-d12	23.28	264	2321695	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	37711	4.47	ng/uL	0.00
5) Phenol-d5	6.71	99	178429	5.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	456547	25.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	490495	21.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	324086	12.81	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	280719	27.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	307234	28.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	572291	23.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.45	131	39339	1.47	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	1982392	29.46	ng/ul	0.00
47) Acenaphthylene-d8	13.86	160	2155613	28.07	ng/ul	0.00
52) 4-Nitrophenol-d4	14.41	143	47049	4.10	ng/ul	0.00
58) Fluorene-d10	15.17	176	1683433	28.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	271327	25.47	ng/ul	0.00
71) Anthracene-d10	17.03	188	2675344	30.62	ng/ul	0.00
79) Pyrene-d10	19.33	212	3138675	31.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	3874857	31.72	ng/ul	0.00

Target Compounds


						Qvalue
6) Phenol	6.73	94	36101	1.105	ng/ul	96
35) 1-Methylnaphthalene	12.19	142	82709	1.464	ng/ul	98
45) Dimethylphthalate	13.65	163	109049	1.654	ng/ul	99
50) Acenaphthene	14.24	153	625107	11.395	ng/ul	98
59) Fluorene	15.23	166	511230	7.759	ng/ul	99
75) Carbazole	17.33	167	102945	1.211	ng/ul	99
77) Fluoranthene	18.99	202	117195	1.078	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM023801.D
Acq On : 19 Nov 2019 17:38
Operator : JU
Sample : K5748-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEHP5

Quant Time: Nov 20 06:57:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

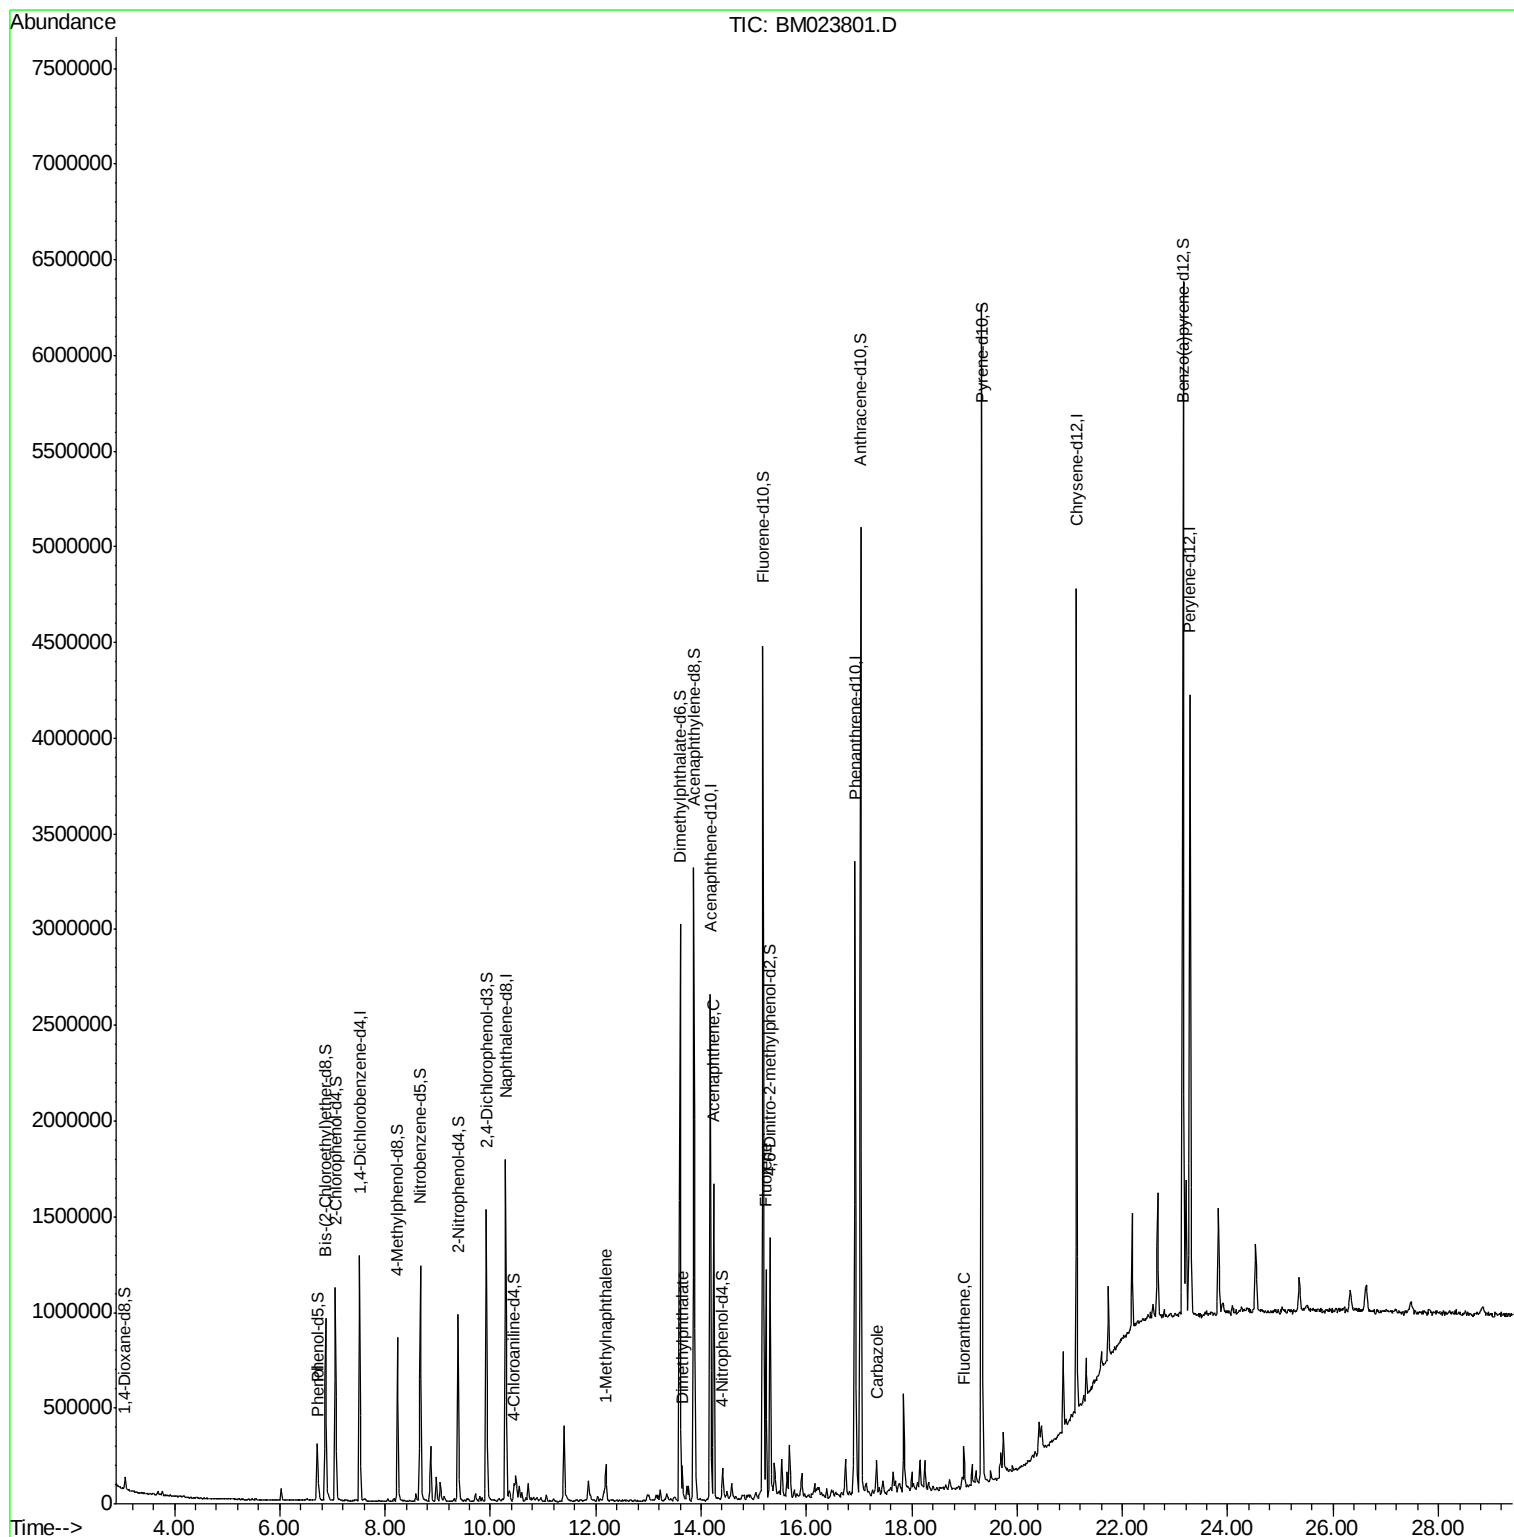

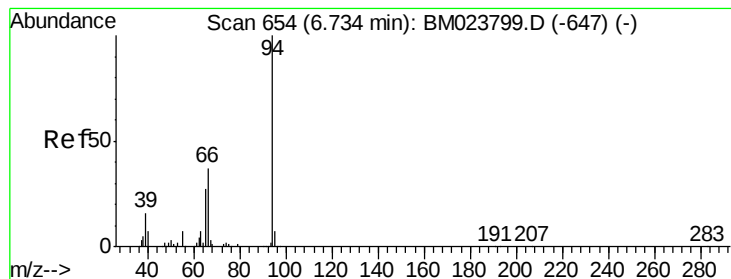

#6

Phenol

Concen: 1.105 ng/ul

RT: 6.73 min Scan# 654

Delta R.T. 0.00 min

Lab File: BM023801.D

Acq: 19 Nov 2019 17:38

Instrument :

BNA_M

ClientSampled :

BEHP5





Tgt Ion: 94 Resp: 36101

Ion Ratio Lower Upper

94 100

65 29.4 21.4 32.2

66 40.3 30.7 46.1

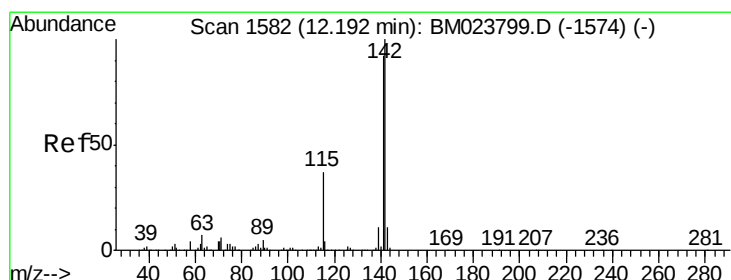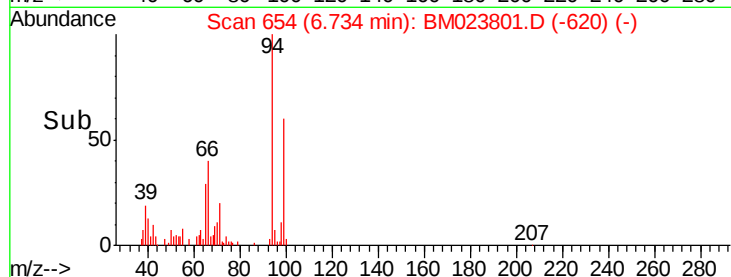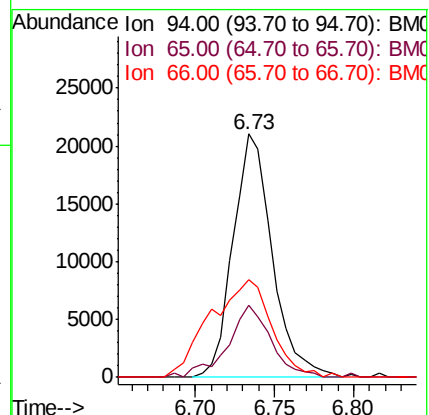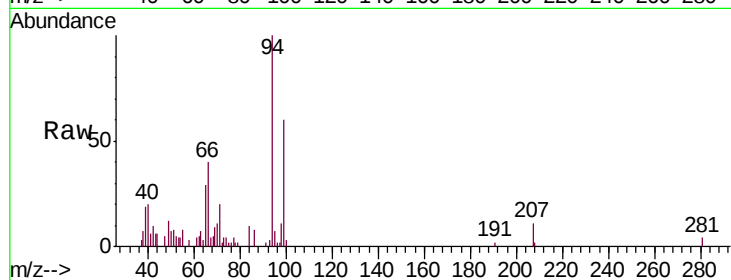

#35

1-Methylnaphthalene

Concen: 1.464 ng/ul

RT: 12.19 min Scan# 1582

Delta R.T. 0.00 min

Lab File: BM023801.D

Acq: 19 Nov 2019 17:38




Tgt Ion: 142 Resp: 82709


Ion Ratio Lower Upper

142 100

141 91.2 74.6 112.0

116 3.8 3.2 4.8

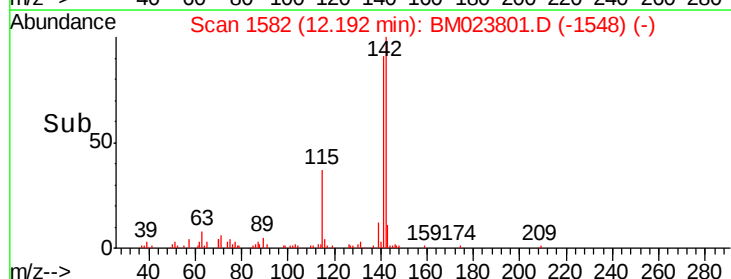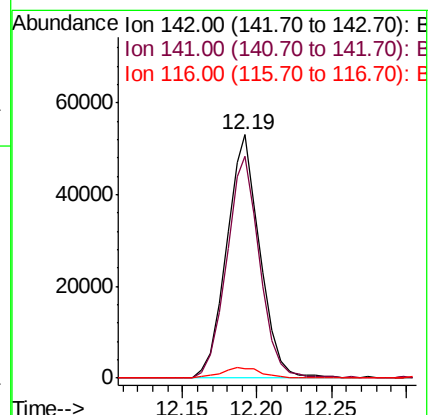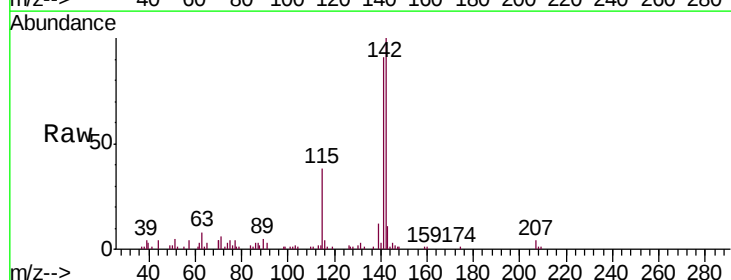

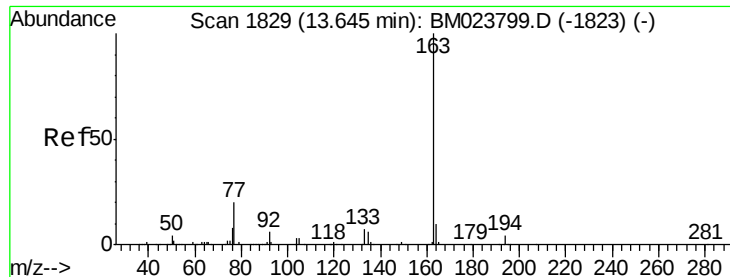

#45

Dimethylphthalate

Concen: 1.654 ng/ul

RT: 13.65 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM023801.D

Acq: 19 Nov 2019 17:38

Instrument :

BNA_M

ClientSampleId :

BEHP5


Tgt Ion:163 Resp: 109049

Ion Ratio Lower Upper

163 100

194 5.0 3.4 5.2




164 9.6 8.0 12.0

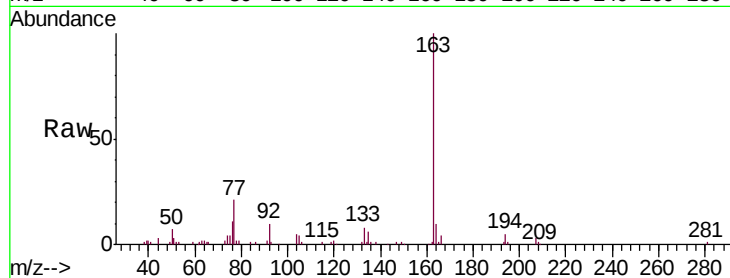

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

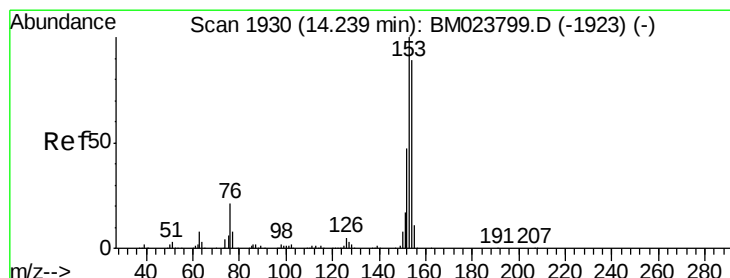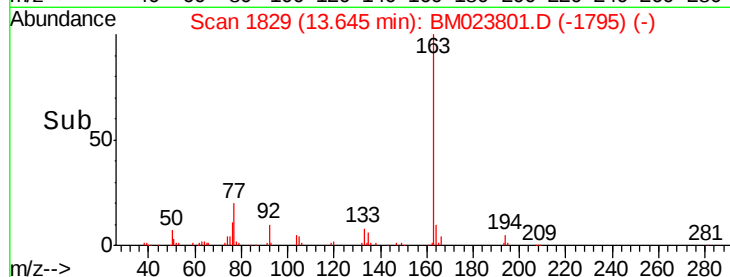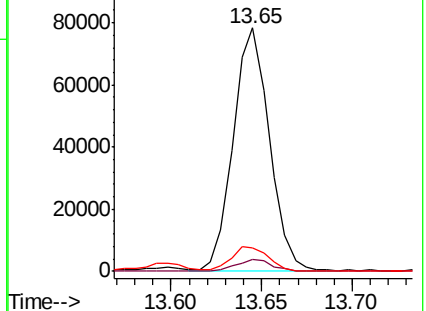

#50

Acenaphthene

Concen: 11.395 ng/ul

RT: 14.24 min Scan# 1930

Delta R.T. 0.00 min

Lab File: BM023801.D

Acq: 19 Nov 2019 17:38


Tgt Ion:153 Resp: 625107

Ion Ratio Lower Upper

153 100

152 48.5 37.7 56.5



154 90.6 70.6 106.0

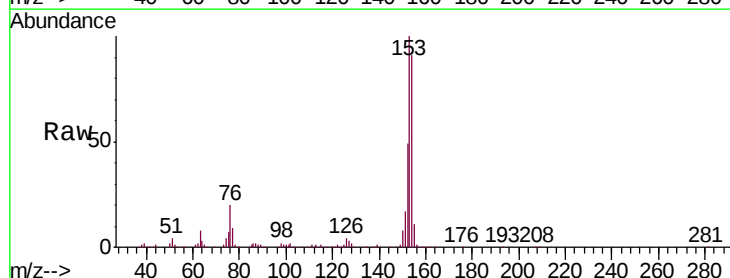


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

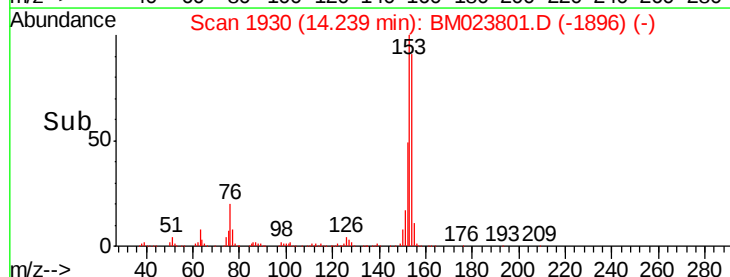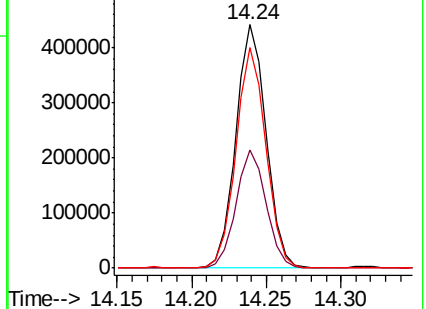

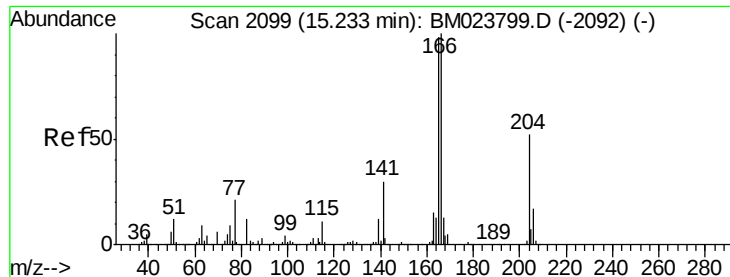

#59

Fluorene

Concen: 7.759 ng/ul

RT: 15.23 min Scan# 2099

Delta R.T. 0.00 min

Lab File: BM023801.D

Acq: 19 Nov 2019 17:38

Instrument :

BNA_M

ClientSampleId :

BEHP5


Tgt Ion:166 Resp: 511230

Ion Ratio Lower Upper

166 100

165 95.8 77.2 115.8




167 15.3 10.9 16.3

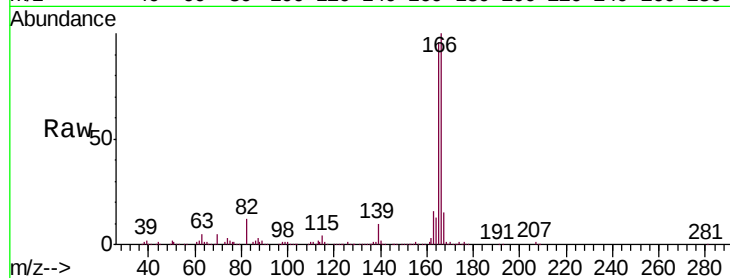

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

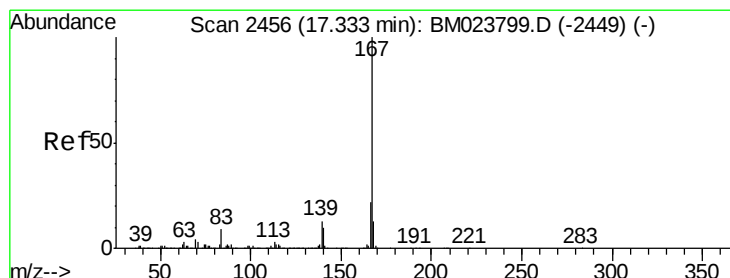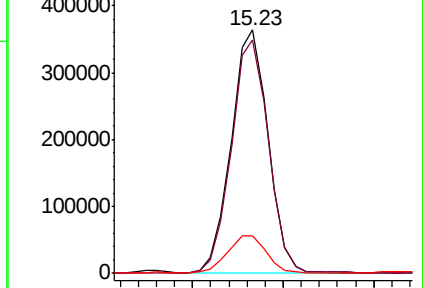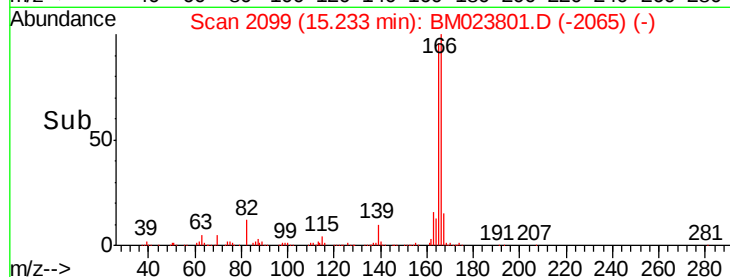

#75

Carbazole

Concen: 1.211 ng/ul

RT: 17.33 min Scan# 2456

Delta R.T. 0.00 min

Lab File: BM023801.D

Acq: 19 Nov 2019 17:38


Tgt Ion:167 Resp: 102945

Ion Ratio Lower Upper

167 100

166 21.5 17.1 25.7



139 13.3 9.8 14.6

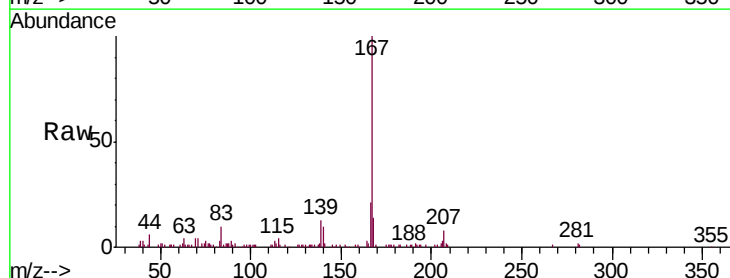


Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

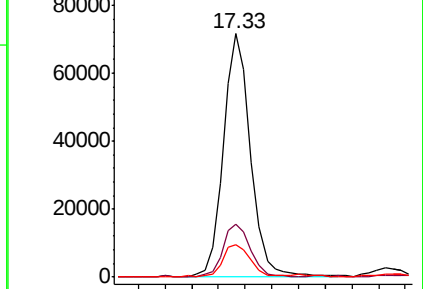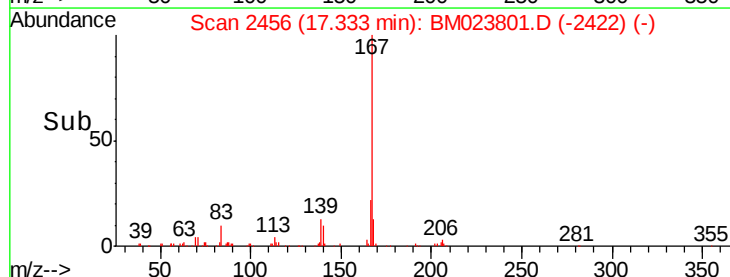

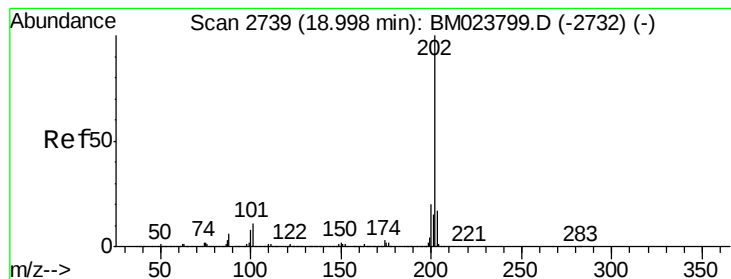

#77

Fluoranthene

Concen: 1.078 ng/ul

RT: 18.99 min Scan# 2738

Delta R.T. -0.01 min

Lab File: BM023801.D

Acq: 19 Nov 2019 17:38

Instrument :

BNA_M

ClientSampleId :

BEHP5



Tgt Ion: 202 Resp: 117195

Ion Ratio Lower Upper

202 100

101 12.2 7.7 11.5#

100 9.6 6.0 9.0#

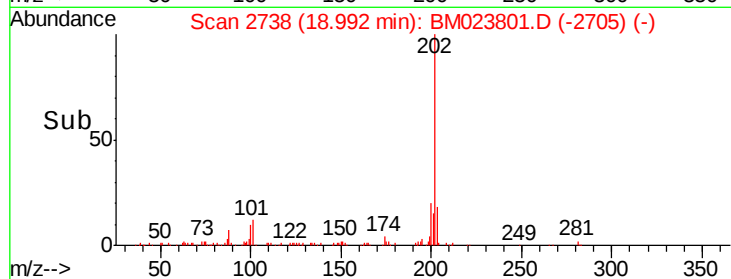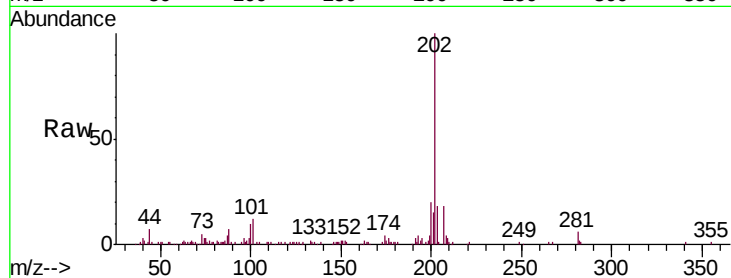

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

