

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111919\
Quantitation Report (QT Reviewed)


Data File : BM023802.D
Acq On : 19 Nov 2019 18:15
Operator : JU
Sample : K5748-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEHP6

Manual Integrations
APPROVED

mohammad
11/21/2019 9:06:33 AM

Quant Time: Nov 20 07:05:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

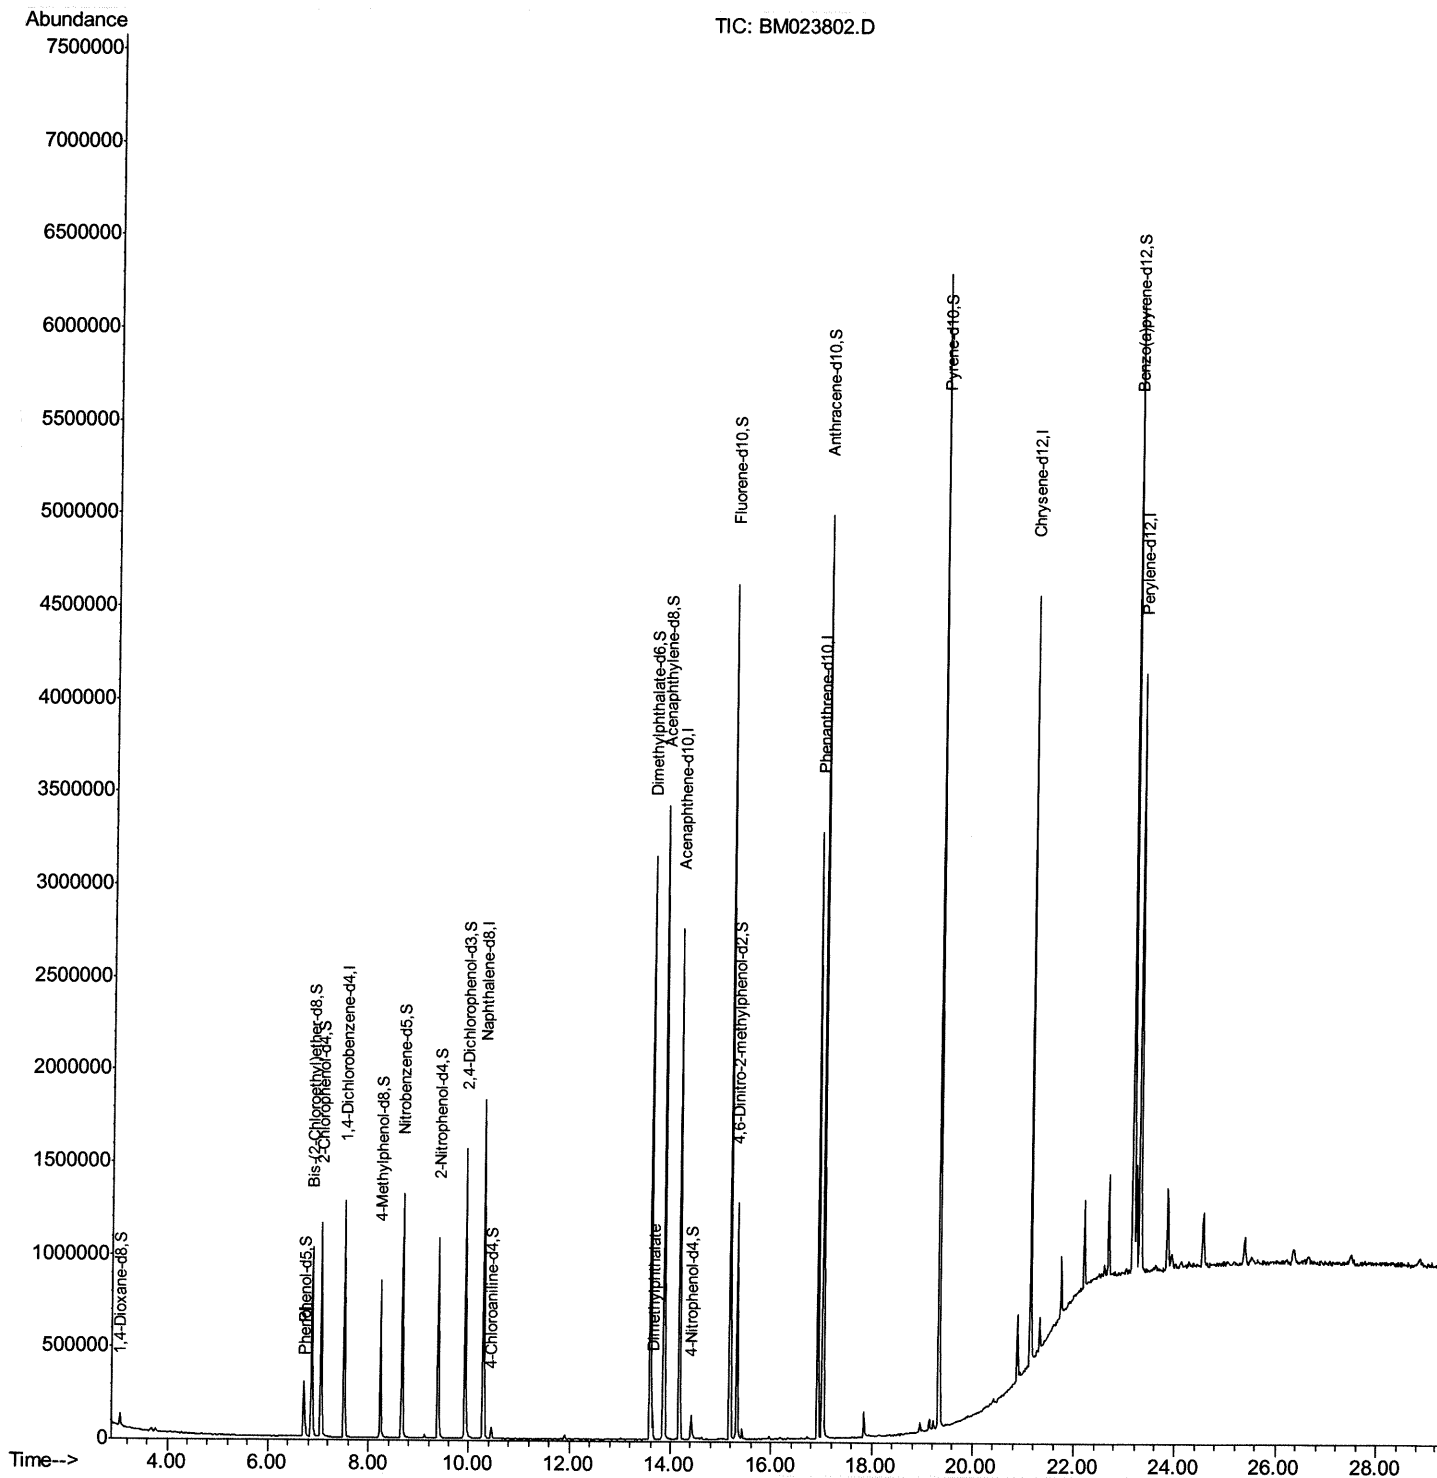

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111919\
Quantitation Report (Qedit)




Data File : BM023802.D
Acq On : 19 Nov 2019 18:15
Operator : JU
Sample : K5748-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEHP6

Manual Integrations
APPROVED

mohammad
11/21/2019 9:06:33 AM

Quant Time: Nov 20 06:57:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

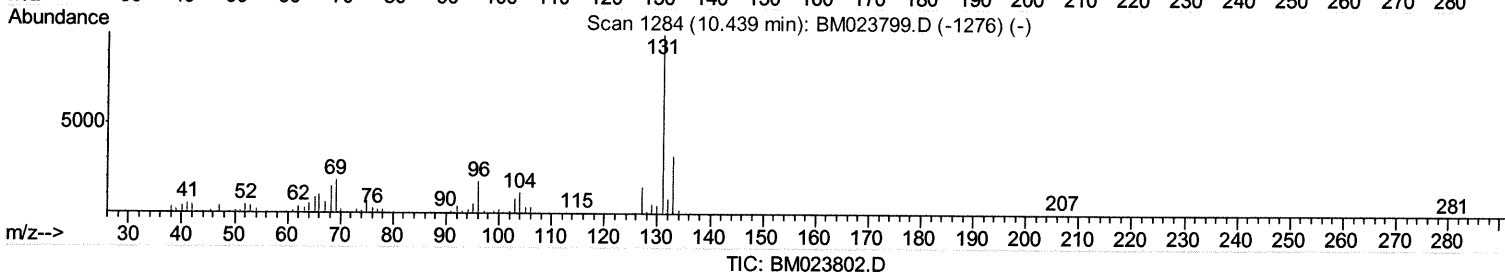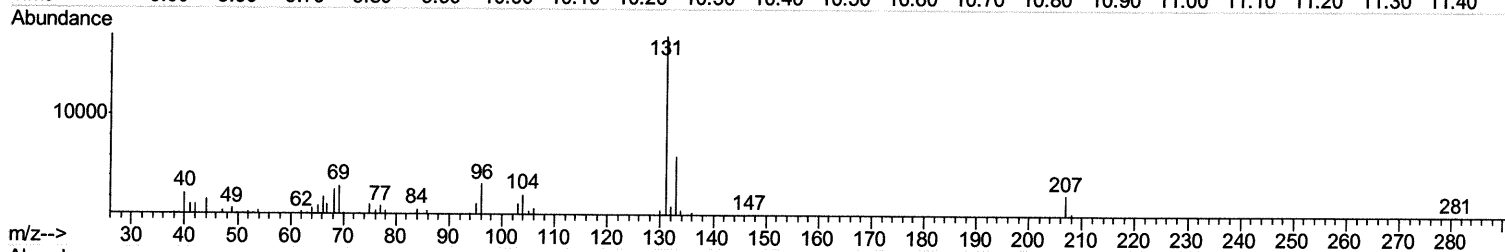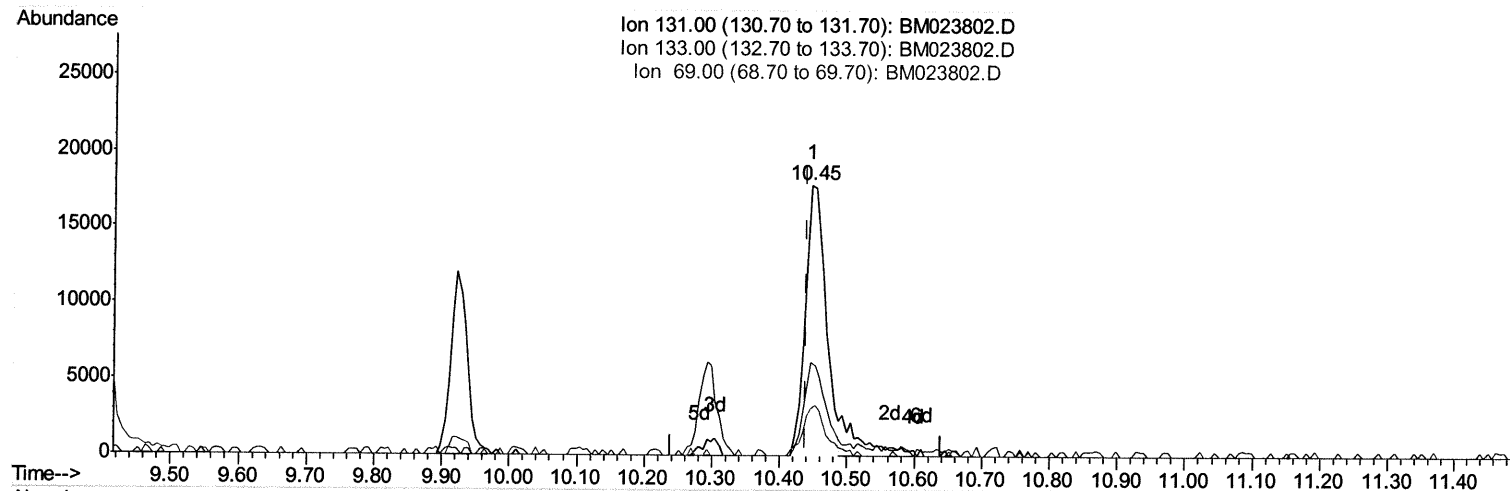

(29) 4-Chloroaniline-d4 (S)

10.445min (+0.006) 1.35ng/ul

response 37265

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	34.42
69.00	19.60	17.26
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111919\
Quantitation Report (Qedit)




Data File : BM023802.D
Acq On : 19 Nov 2019 18:15
Operator : JU
Sample : K5748-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEHP6

Manual Integrations
APPROVED

mohammad
11/21/2019 9:06:33 AM

Quant Time: Nov 20 06:57:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

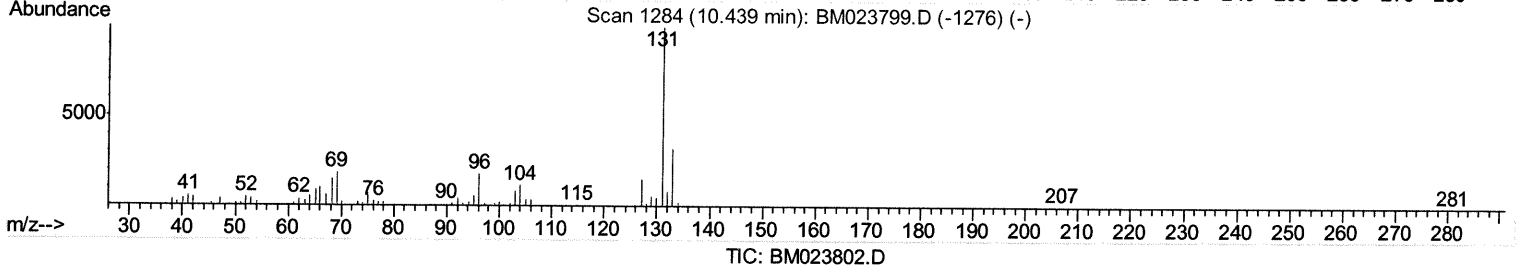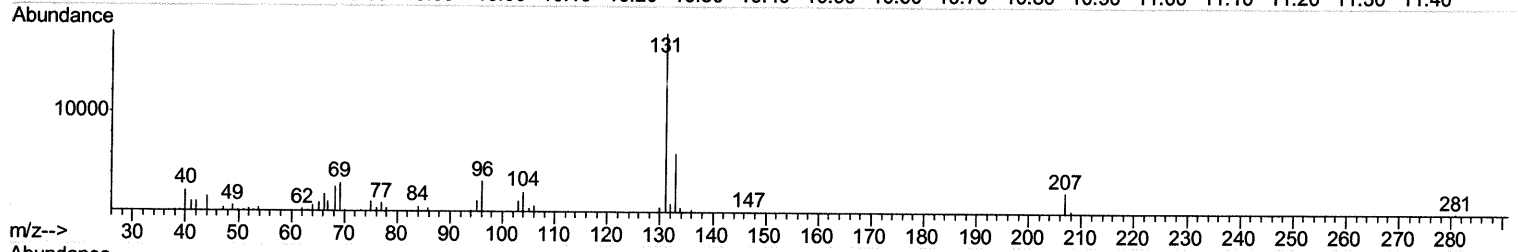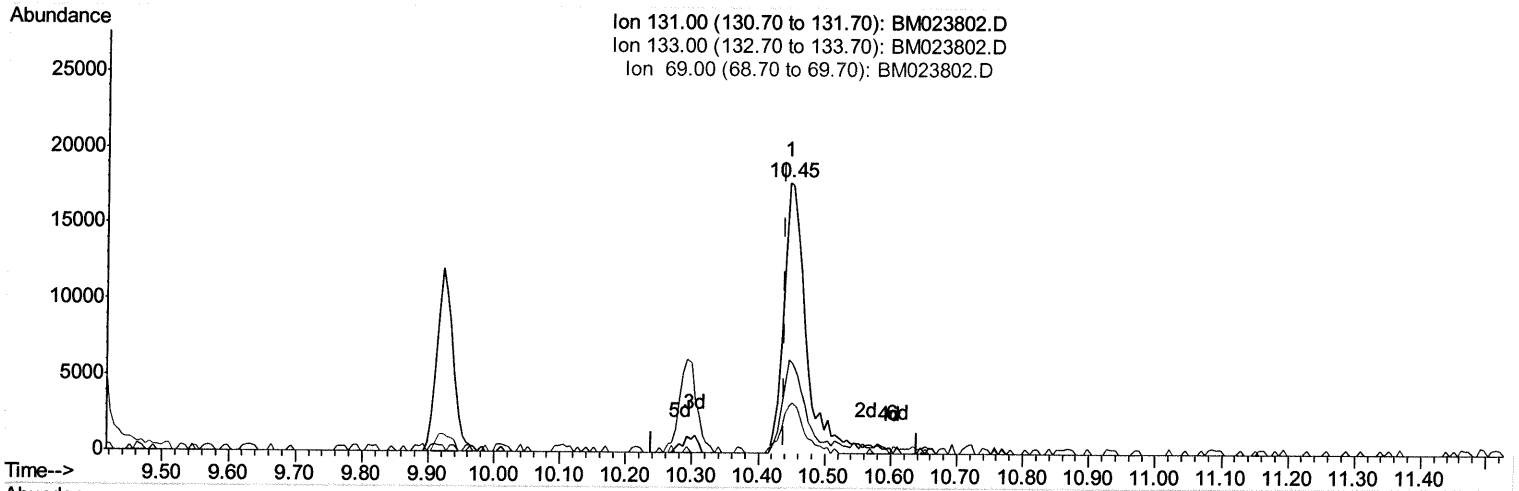

(29) 4-Chloroaniline-d4 (S)

10.445min (+0.006) 1.48ng/ul m

response 40980

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	34.42
69.00	19.60	17.26
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111919\
Quantitation Report (QT Reviewed)

Data File : BM023802.D
Acq On : 19 Nov 2019 18:15
Operator : JU
Sample : K5748-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEHP6

Manual Integrations
APPROVED

mohammad
11/21/2019 9:06:33 AM

Quant Time: Nov 20 07:05:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	350275	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	1465119	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.17	164	898662	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	1855054	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1832185	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	2234625	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	40259	4.74	ng/uL	0.00
5) Phenol-d5	6.71	99	183845	5.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	498088	27.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	515624	22.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	329623	12.94	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	305234	29.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	334141	30.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	592421	23.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.45	131	40980m	1.48	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	2021599	28.85	ng/ul	0.00
47) Acenaphthylene-d8	13.86	160	2270494	28.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.41	143	43946	3.67	ng/ul	0.00
58) Fluorene-d10	15.17	176	1754950	28.36	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	264640	24.66	ng/ul	0.00
71) Anthracene-d10	17.03	188	2763014	31.40	ng/ul	0.00
79) Pyrene-d10	19.33	212	3084049	32.28	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	3696474	31.44	ng/ul	0.00

Target Compounds

					Qvalue
6) Phenol	6.73	94	36748	1.117 ng/ul#	91
45) Dimethylphthalate	13.65	163	92257	1.343 ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed