

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111919\
 Data File : BM023798.D
 Acq On : 19 Nov 2019 15:50
 Operator : JU
 Sample : K5748-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEH01

Quant Time: Nov 19 16:44:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 19 12:27:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	317738	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	1287562	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.17	164	766209	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	1573548	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1546184	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	1901618	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	39833	5.17	ng/uL	0.00
5) Phenol-d5	6.71	99	204961	7.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	534447	32.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	566605	27.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	357570	15.48	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	325233	35.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	353428	36.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.93	165	625191	28.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.45	131	43875	1.81	ng/ul	0.01
44) Dimethylphthalate-d6	13.60	166	2000059	33.47	ng/ul	0.00
47) Acenaphthylene-d8	13.86	160	2309600	33.87	ng/ul	0.00
52) 4-Nitrophenol-d4	14.41	143	42215	4.14	ng/ul	0.00
58) Fluorene-d10	15.17	176	1755184	33.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	244082	26.82	ng/ul	0.00
71) Anthracene-d10	17.03	188	2705725	36.25	ng/ul	0.00
79) Pyrene-d10	19.33	212	3009998	37.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	3650922	36.48	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.64	163	82827	1.415	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111919\
Data File : BM023798.D
Acq On : 19 Nov 2019 15:50
Operator : JU
Sample : K5748-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEH01

Quant Time: Nov 19 16:44:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 19 12:27:28 2019
Response via : Initial Calibration

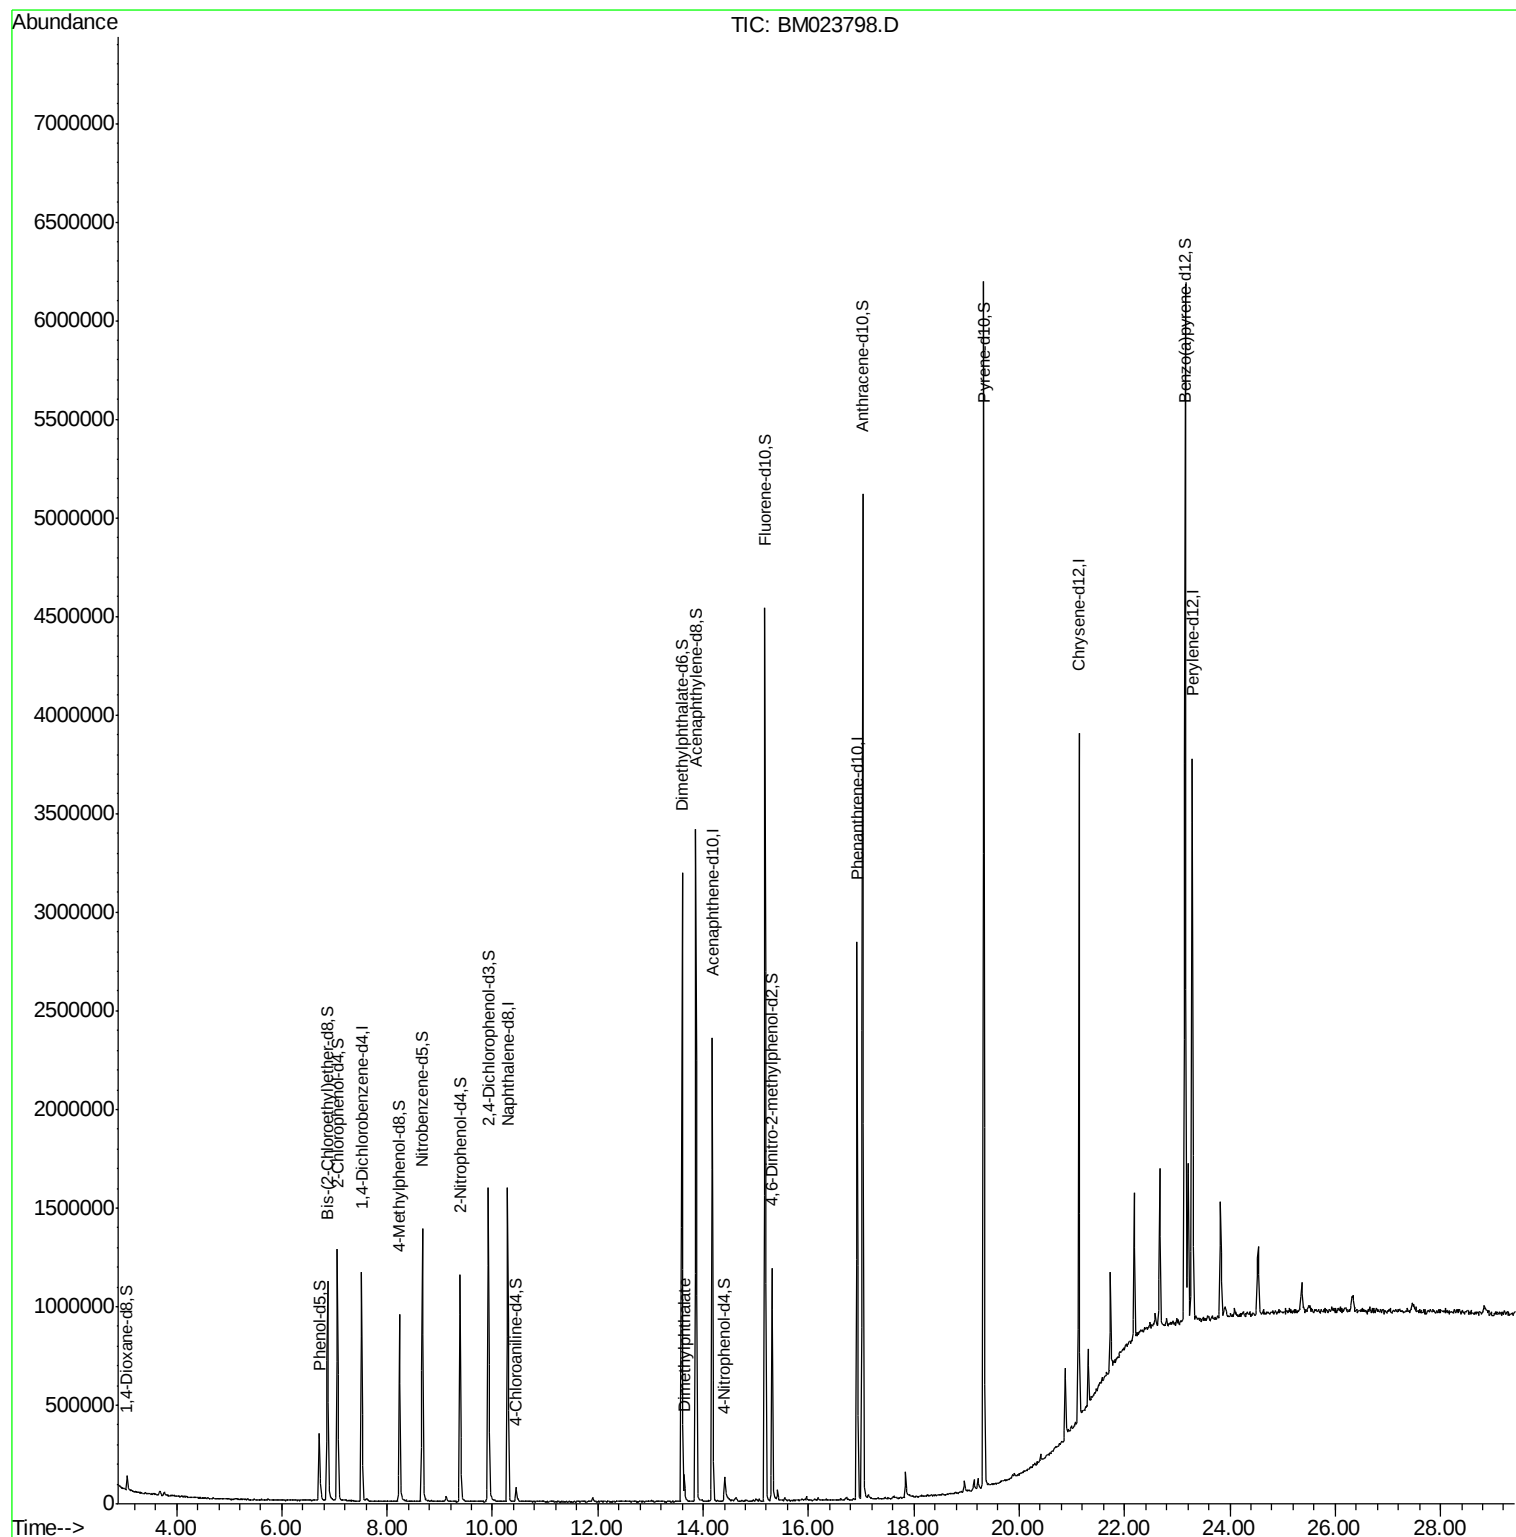

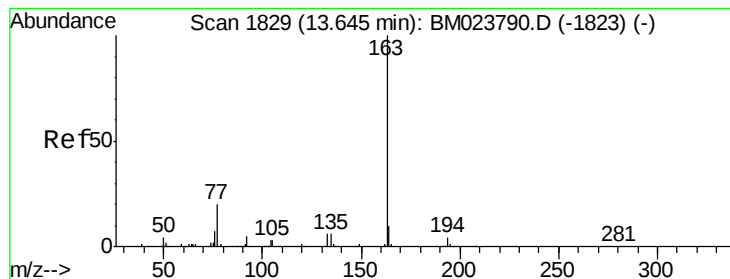

#45

Dimethylphthalate

Concen: 1.415 ng/ul

RT: 13.64 min Scan# 1829

Delta R.T. -0.00 min

Lab File: BM023798.D

Acq: 19 Nov 2019 15:50

Instrument :

BNA_M

ClientSampleId :

BEH01



Tot Ion:163 Resp: 82827

Ion Ratio Lower Upper

163 100

194 4.8 3.4 5.2

164 11.0 8.0 12.0

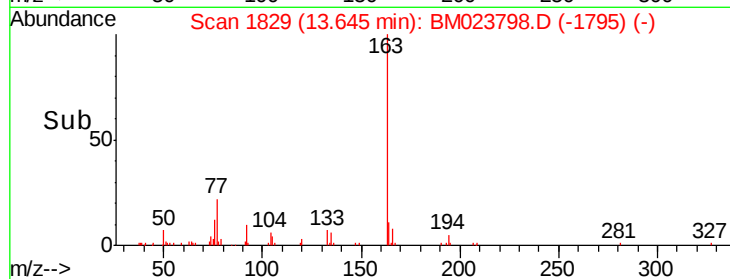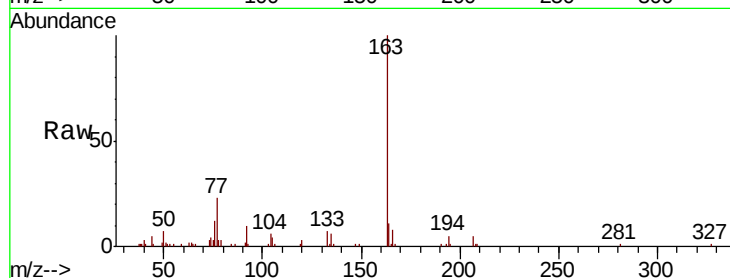

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

