

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111919\
 Data File : BM023805.D
 Acq On : 19 Nov 2019 20:03
 Operator : JU
 Sample : K5748-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEGX6

Quant Time: Nov 20 06:58:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 06:55:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	371953	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	1539700	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.17	164	941790	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	1950872	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1940935	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	2396193	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	42801	4.74	ng/uL	0.00
5) Phenol-d5	6.71	99	208023	6.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	498287	25.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	544276	22.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	381750	14.11	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	310113	28.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	348460	30.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	653938	24.76	ng/ul	0.00
29) 4-Chloroaniline-d4	10.45	131	56547	1.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	2227431	30.33	ng/ul	0.00
47) Acenaphthylene-d8	13.86	160	2437211	29.08	ng/ul	0.00
52) 4-Nitrophenol-d4	14.41	143	54575	4.35	ng/ul	0.00
58) Fluorene-d10	15.17	176	1831337	28.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	297628	26.37	ng/ul	0.00
71) Anthracene-d10	17.03	188	2927809	31.64	ng/ul	0.00
79) Pyrene-d10	19.33	212	3344291	33.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	4145231	32.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.65	163	183488	2.549	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111919\
Data File : BM023805.D
Acq On : 19 Nov 2019 20:03
Operator : JU
Sample : K5748-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEGX6

Quant Time: Nov 20 06:58:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

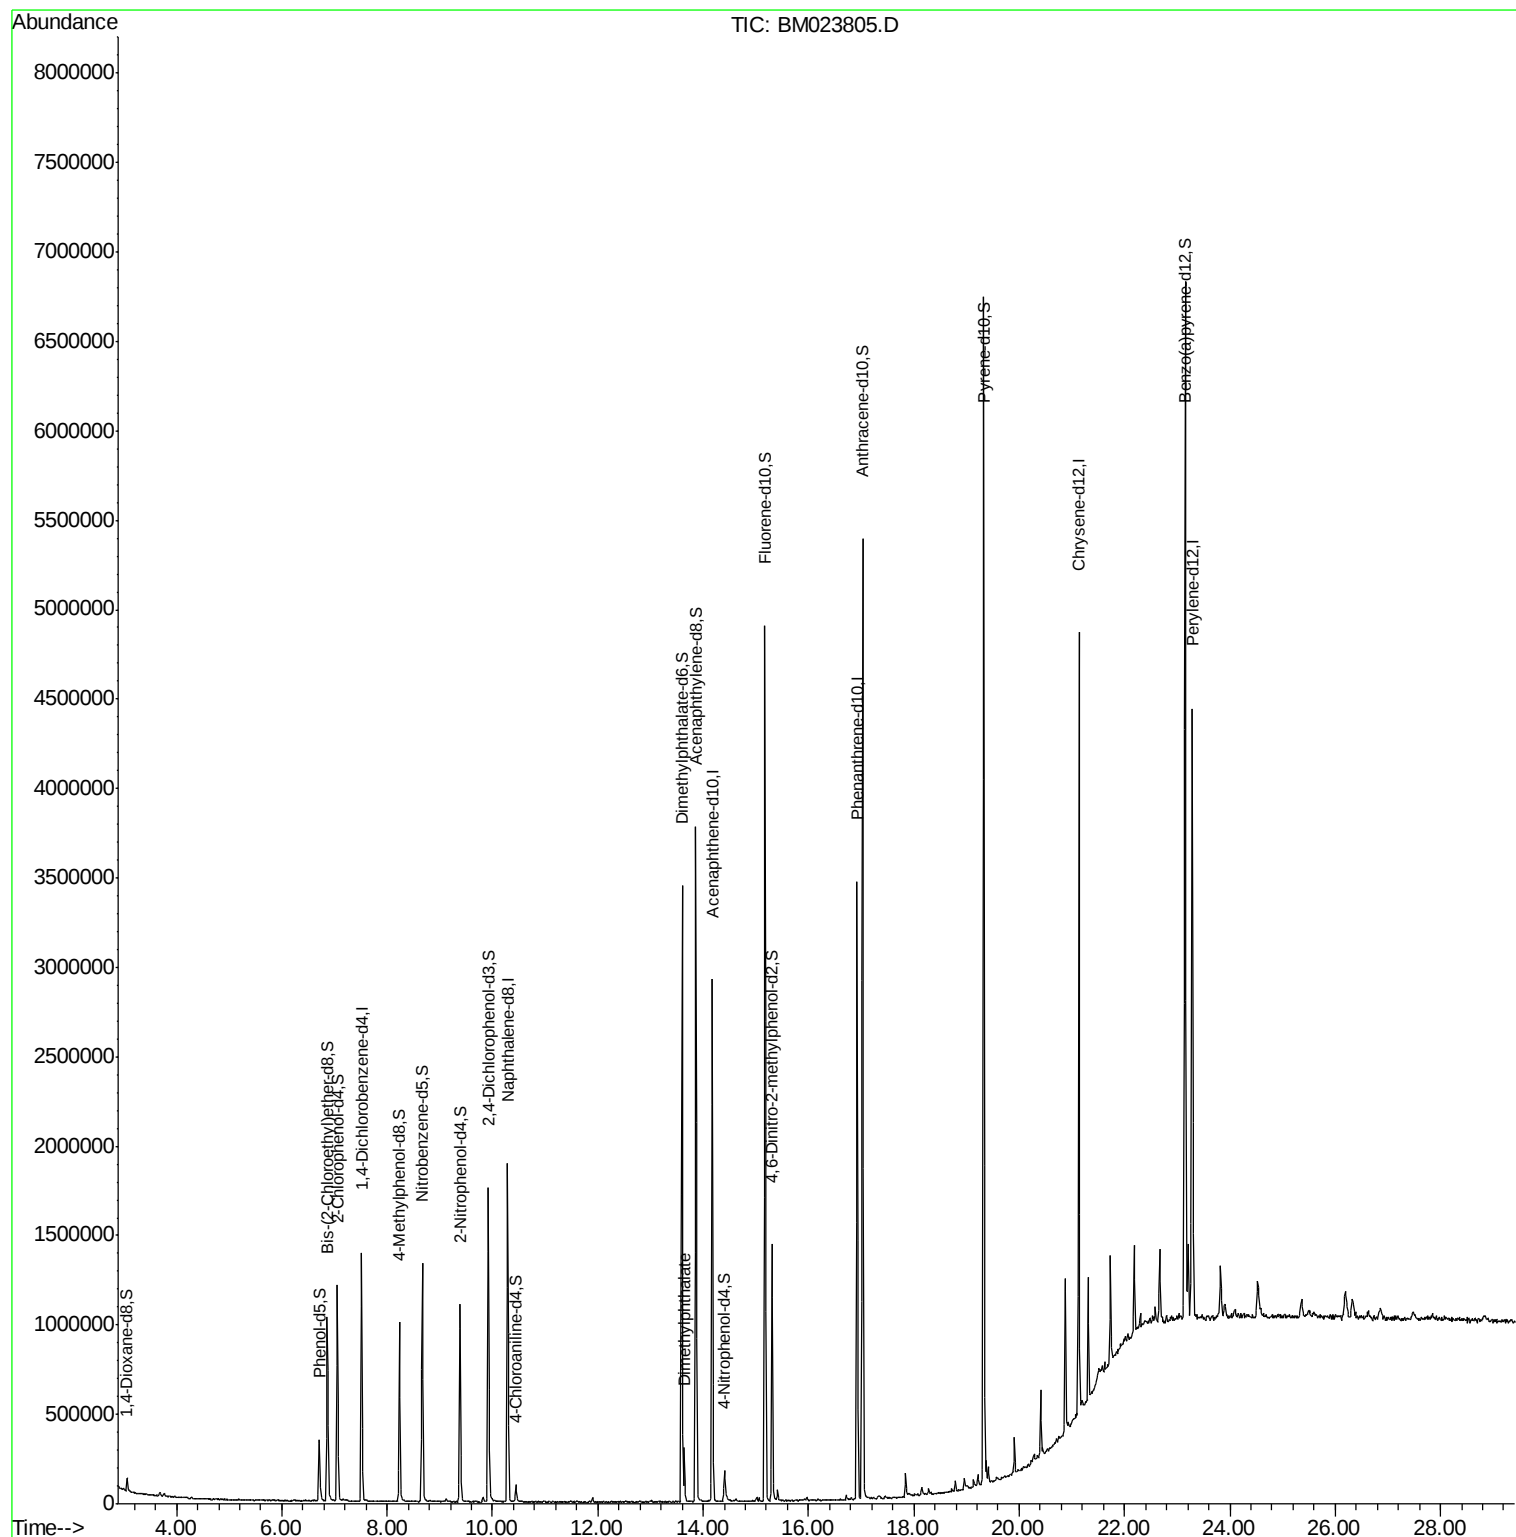

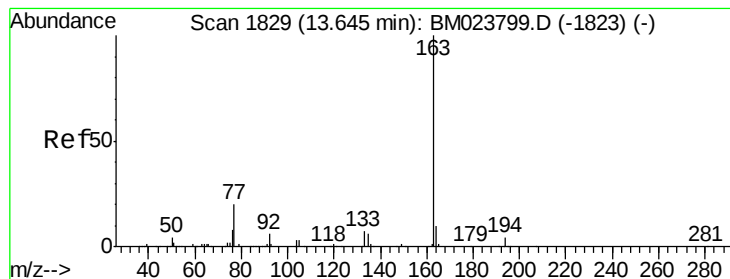

#45

Dimethylphthalate

Concen: 2.549 ng/ul

RT: 13.65 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM023805.D

Acq: 19 Nov 2019 20:03

Instrument :

BNA_M

ClientSampleId :

BEGX6


Tot Ion:163 Resp: 183488

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 9.2 8.0 12.0

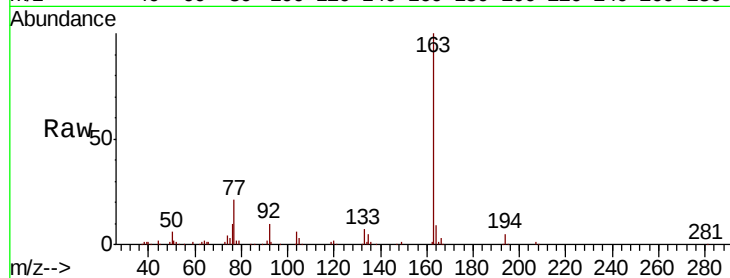

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

