

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111919\
 Data File : BM023819.D
 Acq On : 20 Nov 2019 05:07
 Operator : JU
 Sample : K5847-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFPS3

Quant Time: Nov 20 08:43:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 06:55:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	426046	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	1577853	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	837536	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	1531158	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	1601620	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	2100564	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0d	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0d	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0d	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0d	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0d	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0d	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul
58) Fluorene-d10	0.00	176	0d	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0d	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds					Ovalue
34) 2-Methylnaphthalene	11.97	142	82000	1.293	ng/ul 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111919\
Data File : BM023819.D
Acq On : 20 Nov 2019 05:07
Operator : JU
Sample : K5847-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFPS3

Quant Time: Nov 20 08:43:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 06:55:09 2019
Response via : Initial Calibration

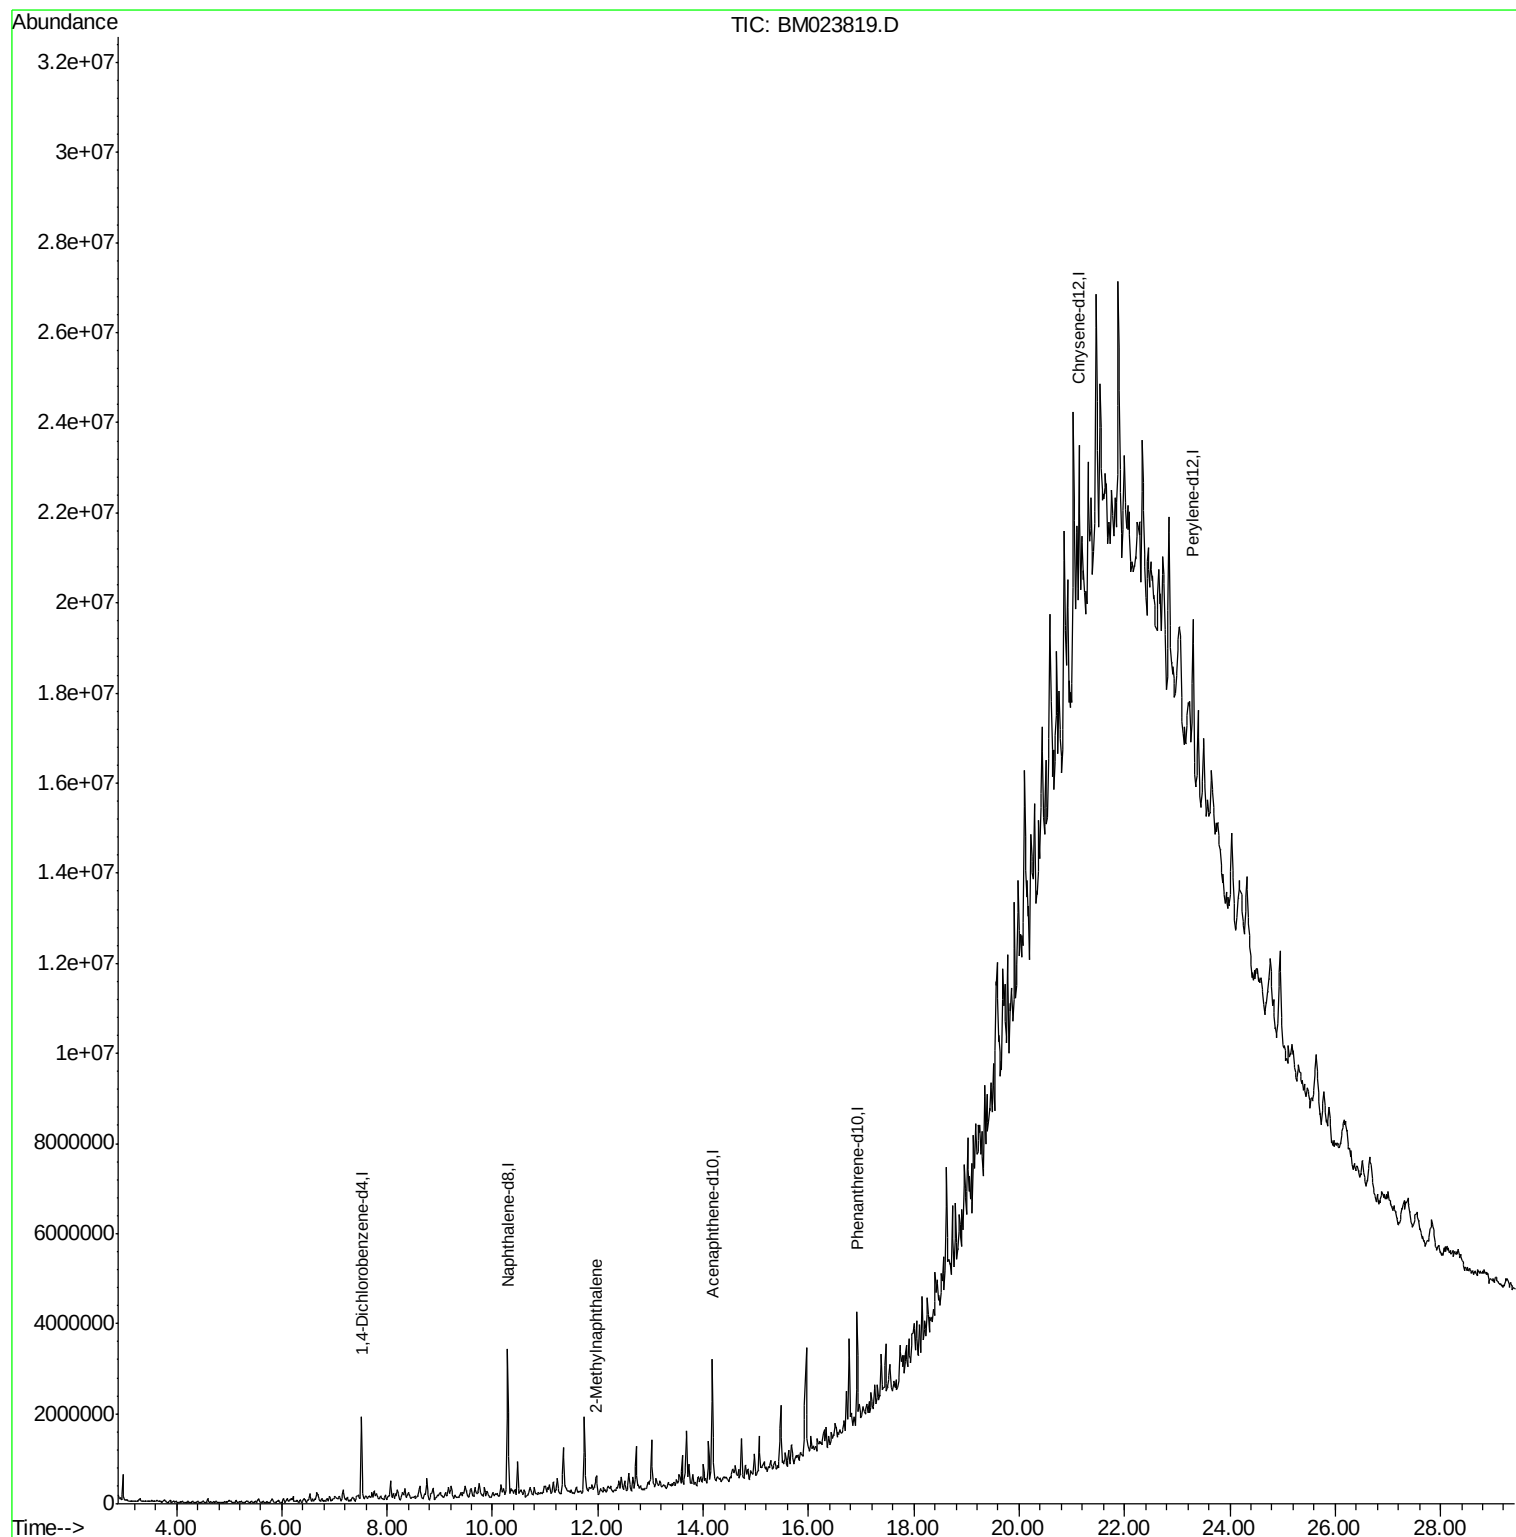

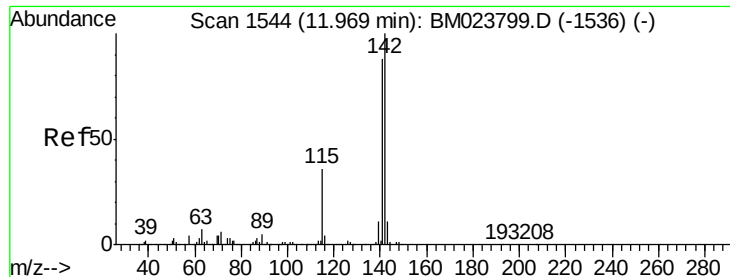

#34

2-Methylnaphthalene

Concen: 1.293 ng/ul

RT: 11.97 min Scan# 1544

Delta R.T. 0.00 min

Lab File: BM023819.D

Acq: 20 Nov 2019 05:07

Instrument :

BNA_M

ClientSampleId :

BFPS3

Tot Ion:142 Resp: 82000

Ion Ratio Lower Upper

142 100

141 91.5 69.8 104.8

