

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111921\
 Data File : BM033188.D
 Acq On : 19 Nov 2021 22:29
 Operator : CG/JU
 Sample : M4677-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB5

Quant Time: Nov 20 01:05:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 19 15:41:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	2605	0.400	ng/ul	0.00
4) Naphthalene-d8	10.760	136	7547	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.580	164	4509	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.316	188	8858	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.470	240	8573	0.400	ng/ul	# 0.00
23) Perylene-d12	23.808	264	8434	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.417	96	12050	4.919	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	3990	0.382	ng/ul	0.00
18) Fluoranthene-d10	19.331	212	11110	0.447	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.962	266	260	0.088	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111921\
Data File : BM033188.D
Acq On : 19 Nov 2021 22:29
Operator : CG/JU
Sample : M4677-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB5


Quant Time: Nov 20 01:05:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 15:41:12 2021
Response via : Initial Calibration

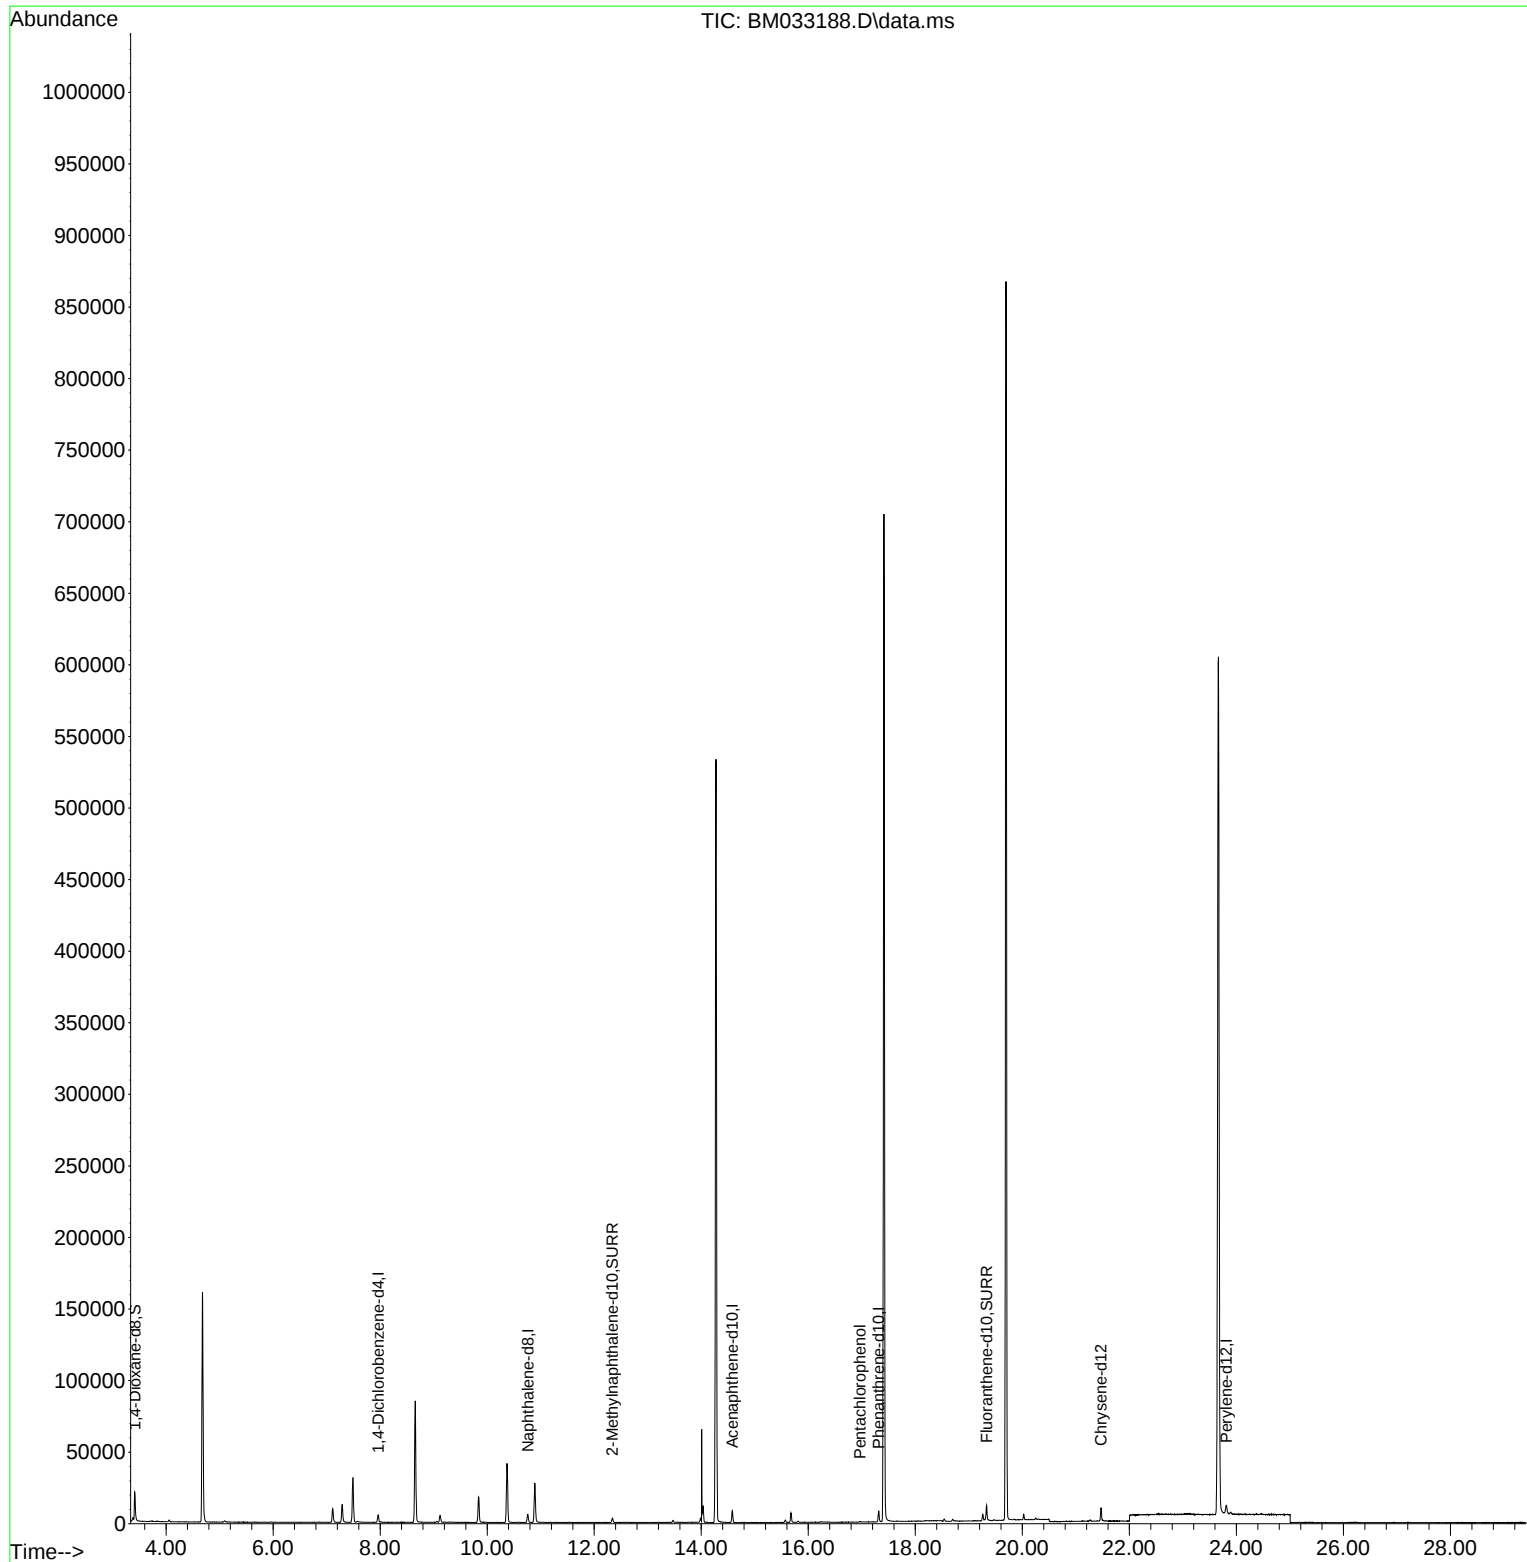

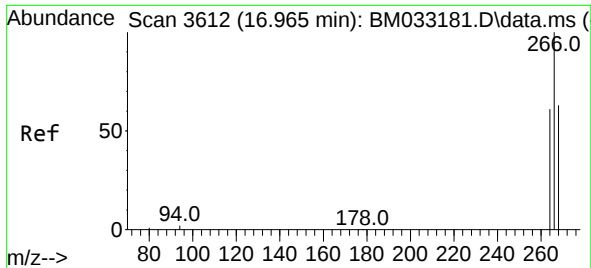

#14
Pentachlorophenol
Concen: 0.088 ng/ul
RT: 16.962 min Scan# 30
Delta R.T. -0.003 min
Lab File: BM033188.D
Acq: 19 Nov 2021 22:29

Instrument :
BNA_M
ClientSampleId :
H0AB5

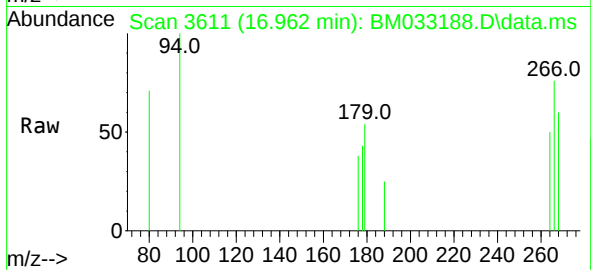

Tgt Ion:	266	Resp:	260
Ion	Ratio	Lower	Upper
266	100		
264	58.8	51.2	76.8
268	65.4	52.9	79.3

