

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111921\
 Data File : BM033193.D
 Acq On : 20 Nov 2021 01:29
 Operator : CG/JU
 Sample : M4677-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB4

Quant Time: Nov 20 02:52:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 19 15:41:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	2962	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	9212	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.580	164	6107	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.316	188	13641	0.400	ng/ul	0.00
17) Chrysene-d12	21.468	240	12950	0.400	ng/ul	# 0.00
23) Perylene-d12	23.808	264	11505	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.413	96	11828	4.247	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	4866	0.381	ng/ul	0.00
18) Fluoranthene-d10	19.331	212	17906	0.477	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.959	266	265	0.058	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111921\
Data File : BM033193.D
Acq On : 20 Nov 2021 01:29
Operator : CG/JU
Sample : M4677-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB4


Quant Time: Nov 20 02:52:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 15:41:12 2021
Response via : Initial Calibration

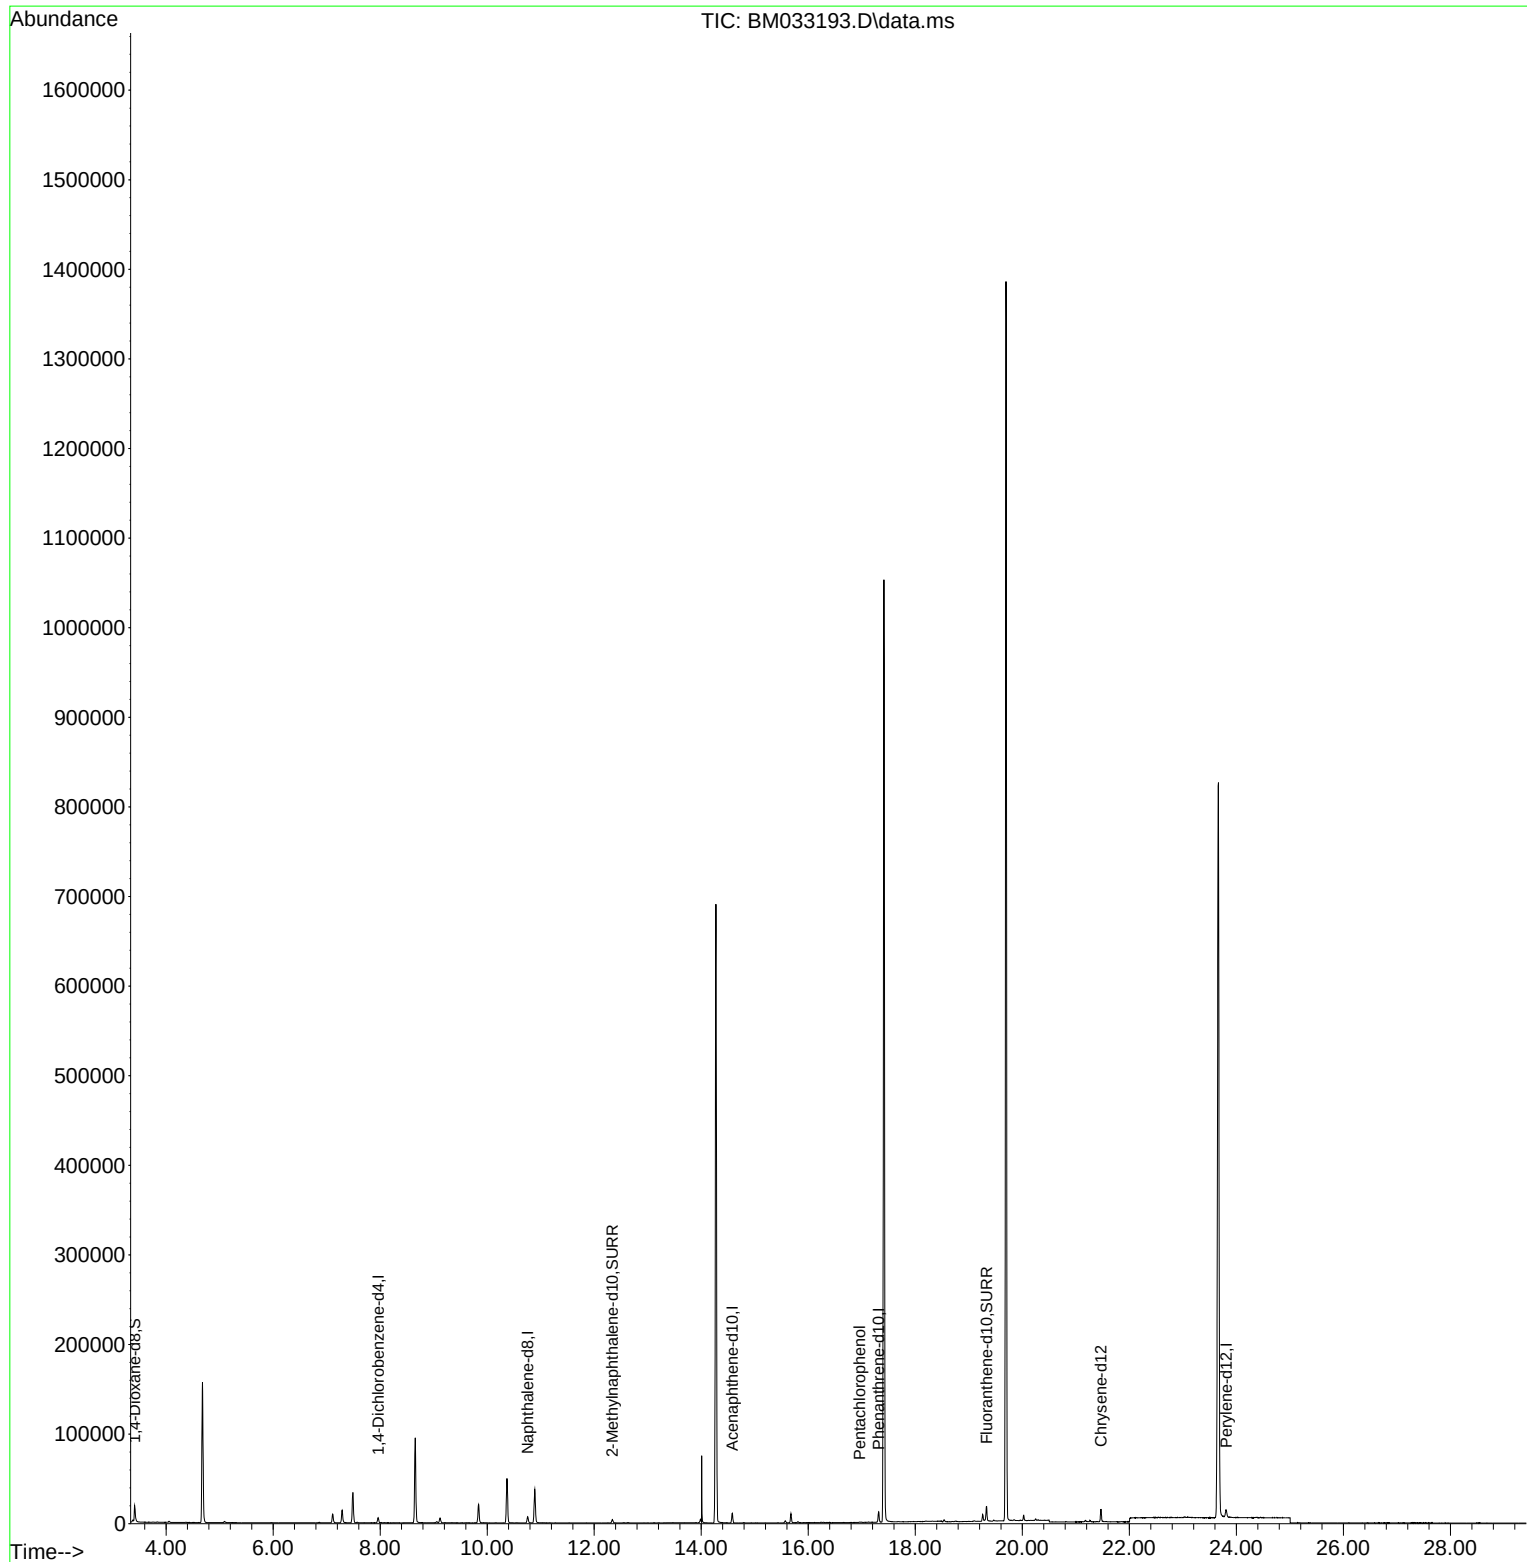

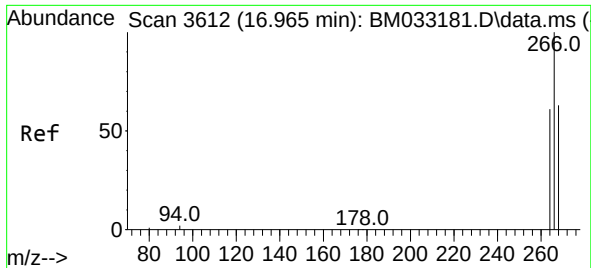

#14
 Pentachlorophenol
 Concen: 0.058 ng/ul
 RT: 16.959 min Scan# 30
 Delta R.T. -0.007 min
 Lab File: BM033193.D
 Acq: 20 Nov 2021 01:29

Instrument :
 BNA_M
 ClientSampleId :
 H0AB4

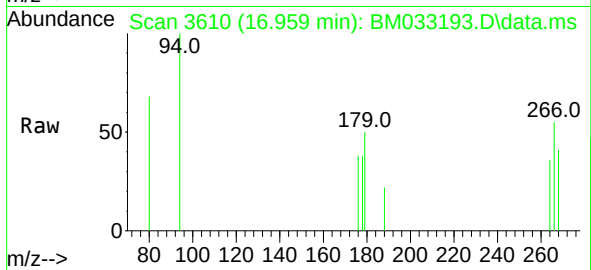

Tgt Ion:	266	Resp:	265
Ion	Ratio	Lower	Upper
266	100		
264	61.5	51.2	76.8
268	67.9	52.9	79.3

