

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111921\
 Data File : BM033195.D
 Acq On : 20 Nov 2021 02:40
 Operator : CG/JU
 Sample : M4677-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AB1

Quant Time: Nov 20 04:03:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 19 15:41:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.960	152	3150	0.400	ng/ul	0.00
4) Naphthalene-d8	10.755	136	9756	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.579	164	6473	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.312	188	13605	0.400	ng/ul	0.00
17) Chrysene-d12	21.467	240	10223	0.400	ng/ul	0.00
23) Perylene-d12	23.804	264	8375	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.413	96	12480	4.213	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.338	152	5390	0.399	ng/ul	0.00
18) Fluoranthene-d10	19.329	212	16760	0.566	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.455	88	359	0.108	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111921\
Data File : BM033195.D
Acq On : 20 Nov 2021 02:40
Operator : CG/JU
Sample : M4677-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AB1

Quant Time: Nov 20 04:03:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 15:41:12 2021
Response via : Initial Calibration

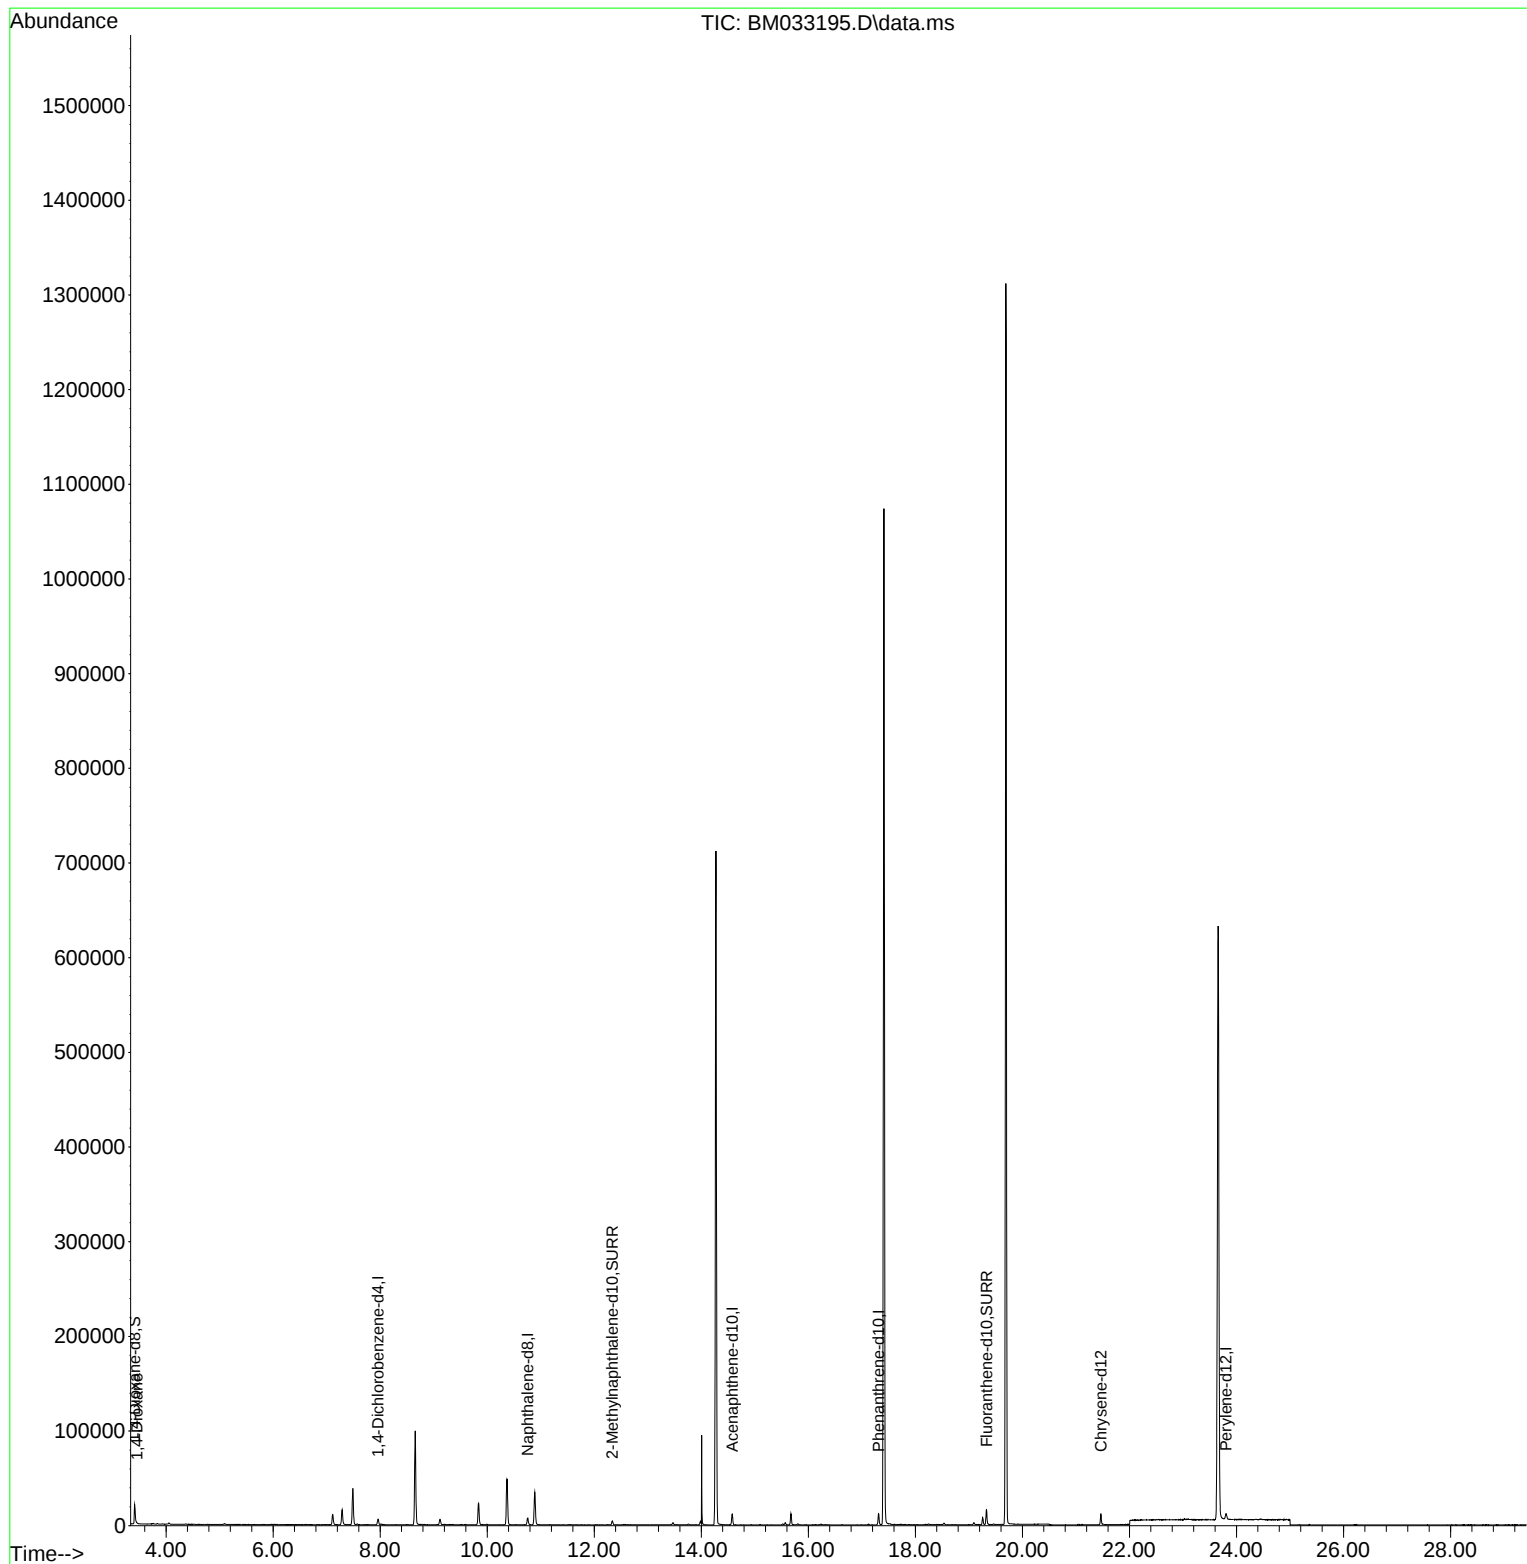

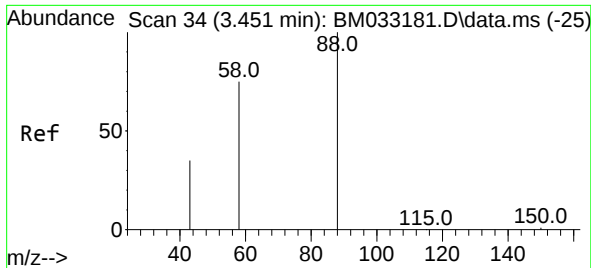

#2
 1,4-Dioxane
 Concen: 0.108 ng/ul
 RT: 3.455 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BM033195.D
 Acq: 20 Nov 2021 02:40

Instrument :
 BNA_M
 ClientSampleId :
 H0AB1

Tgt Ion: 88 Resp: 359
 Ion Ratio Lower Upper
 88 100
 43 81.8 35.8 53.8#
 58 44.2 55.8 83.8#

