
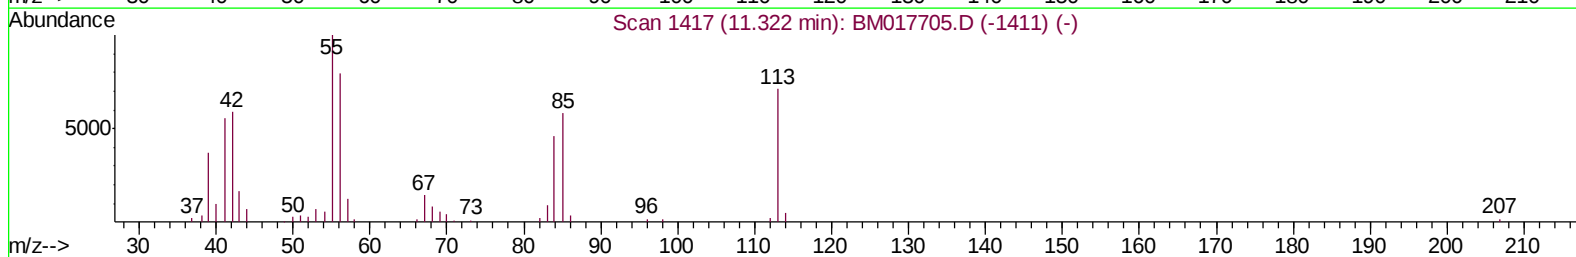
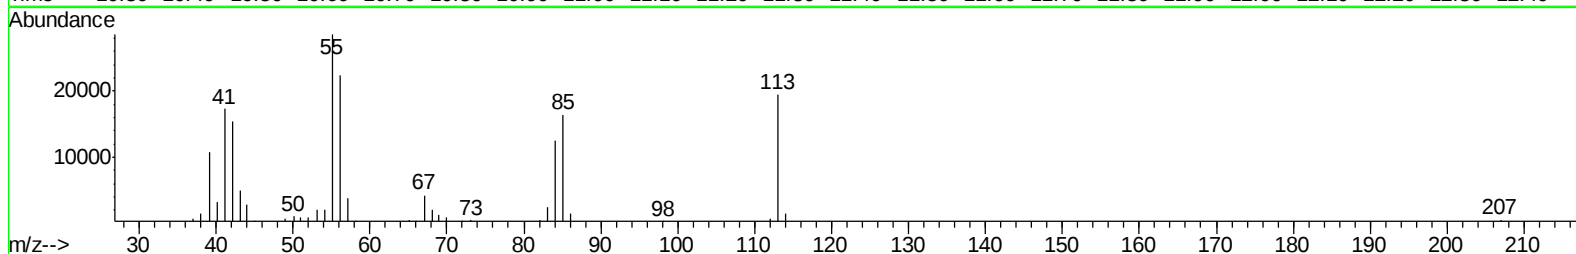


Data File : BM017721.D
Acq On : 21 Nov 2018 01:41
Operator : MJ/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Nov 21 07:42:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 21 01:07:57 2018
Response via : Initial Calibration

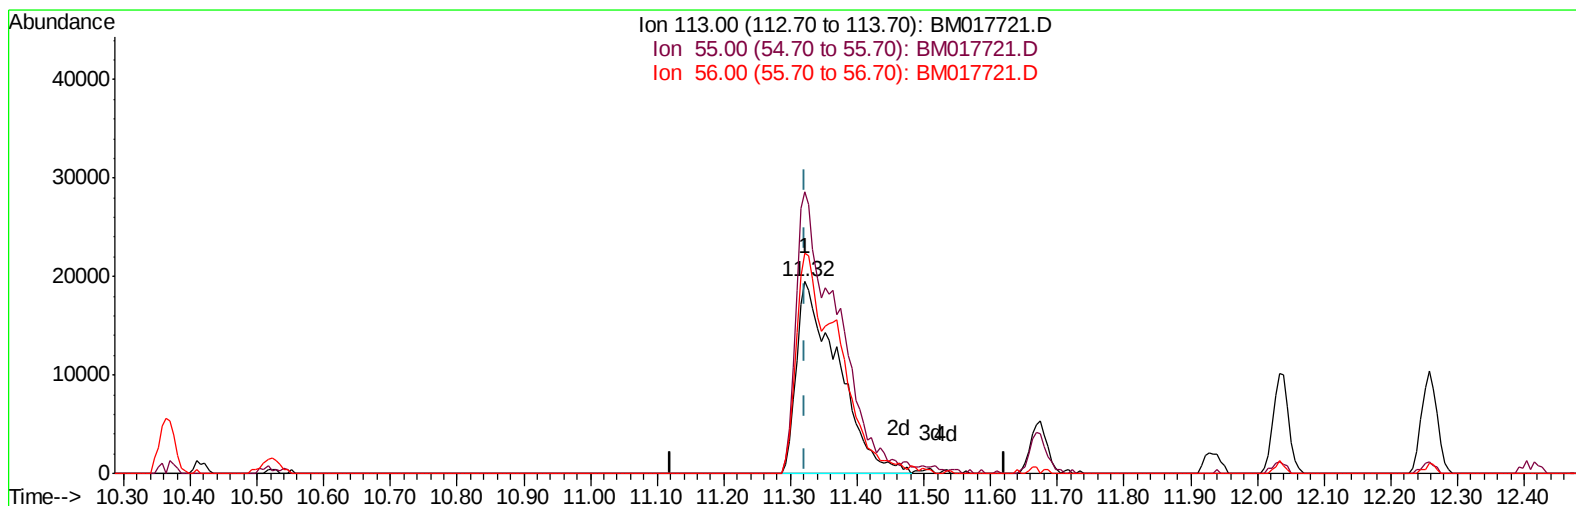

TIC: BM017721.D

(32) Caprolactam

11.322min (+0.000) 19.10ng/ul m

response 83728

Ion	Exp%	Act%
113.00	100	100
55.00	138.30	146.74
56.00	110.30	114.98
0.00	0.00	0.00