
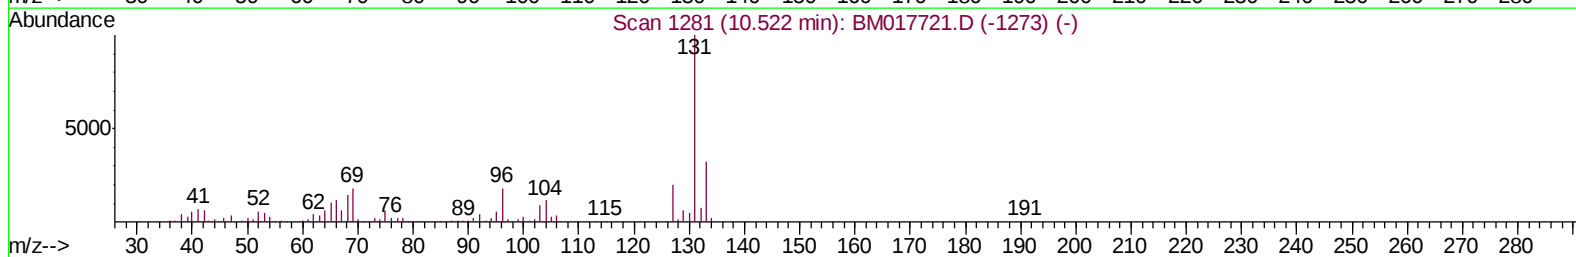
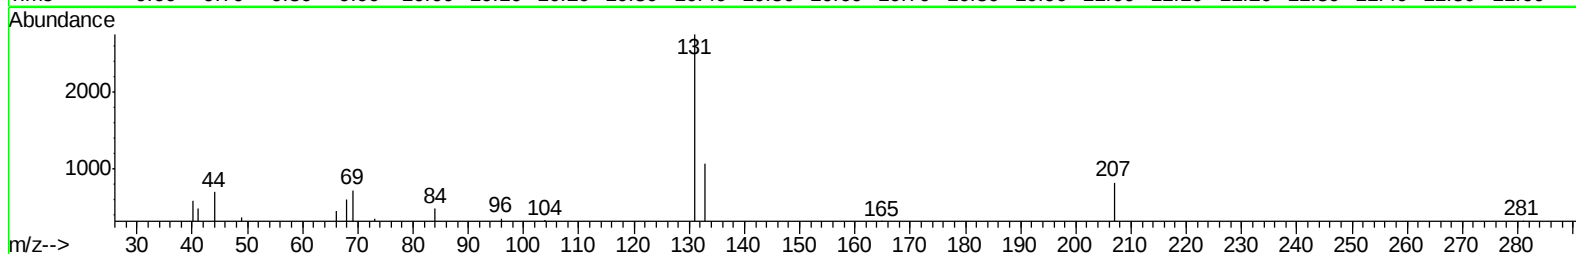


Data File : BM017723.D
Acq On : 21 Nov 2018 02:53
Operator : MJ/SJ
Sample : J5990-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Nov 21 07:46:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 21 07:44:17 2018
Response via : Initial Calibration

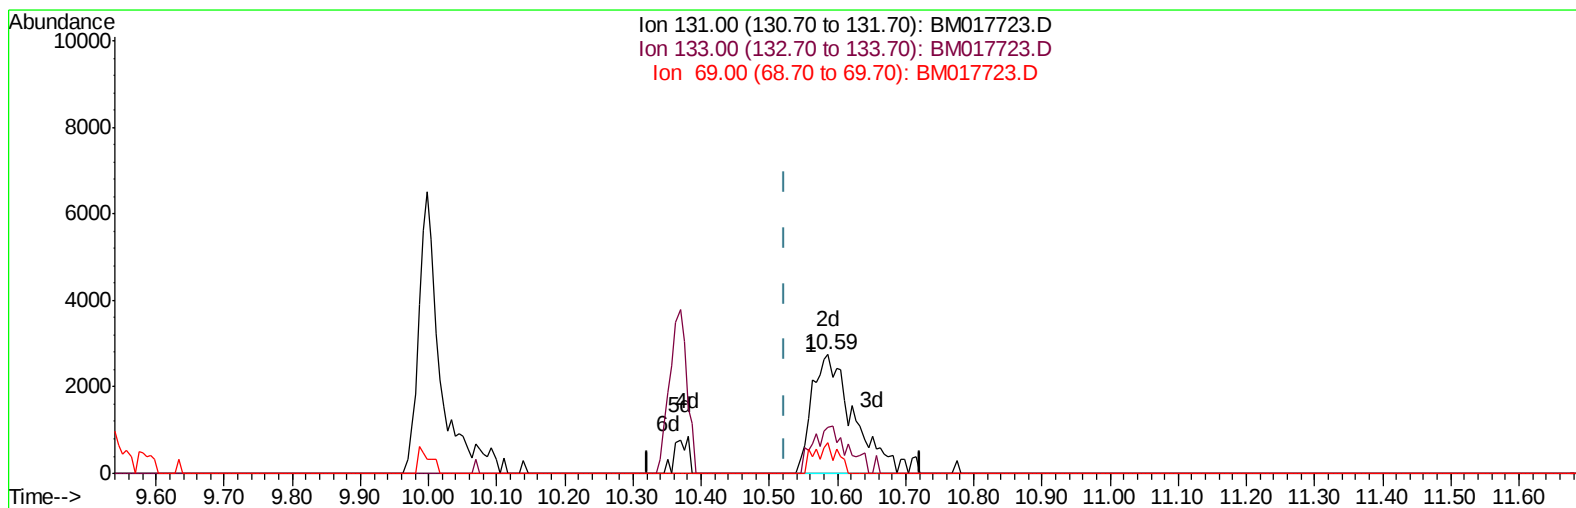

TIC: BM017723.D

(29) 4-Chloroaniline-d4 (S)

10.586min (+0.065) 0.92ng/ul m

response 11474

Ion	Exp%	Act%
131.00	100	100
133.00	32.40	38.75
69.00	18.90	26.25#
0.00	0.00	0.00