
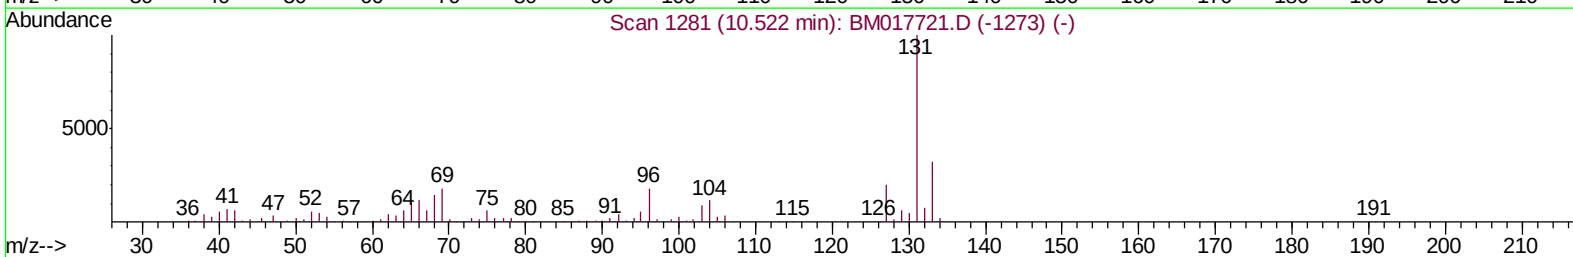
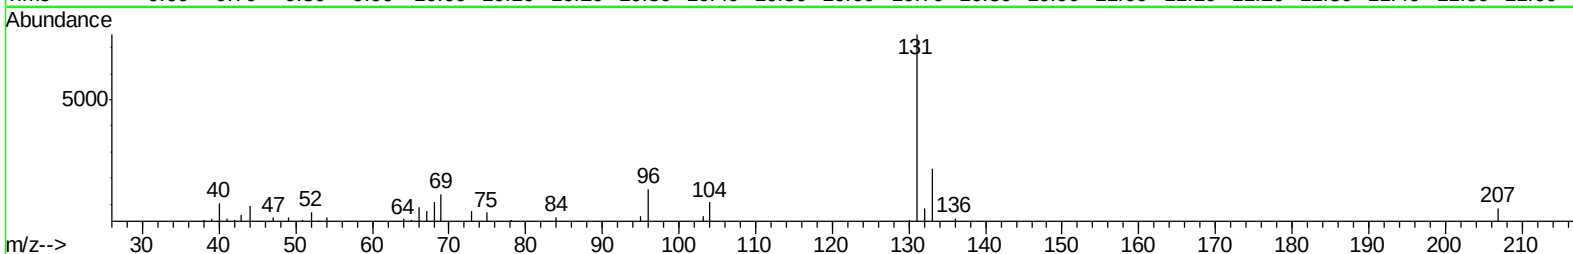


Data File : BM017724.D
Acq On : 21 Nov 2018 03:29
Operator : MJ/SJ
Sample : J5990-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Nov 21 07:47:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 21 07:44:17 2018
Response via : Initial Calibration

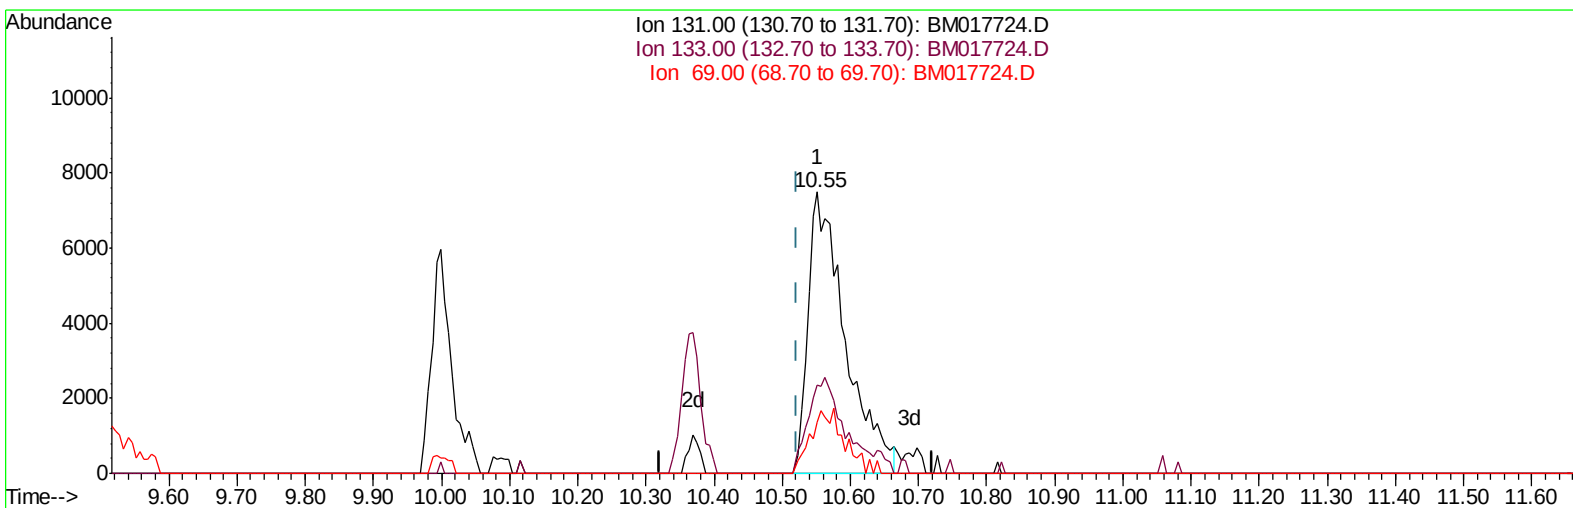

TIC: BM017724.D

(29) 4-Chloroaniline-d4 (S)

10.551min (+0.030) 2.13ng/ul m

response 28351

Ion	Exp%	Act%
131.00	100	100
133.00	32.40	31.41
69.00	18.90	18.31
0.00	0.00	0.00