
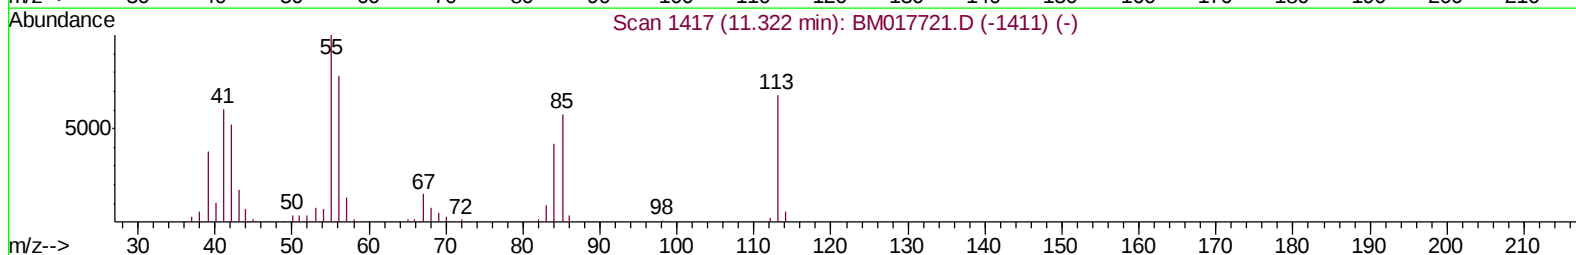
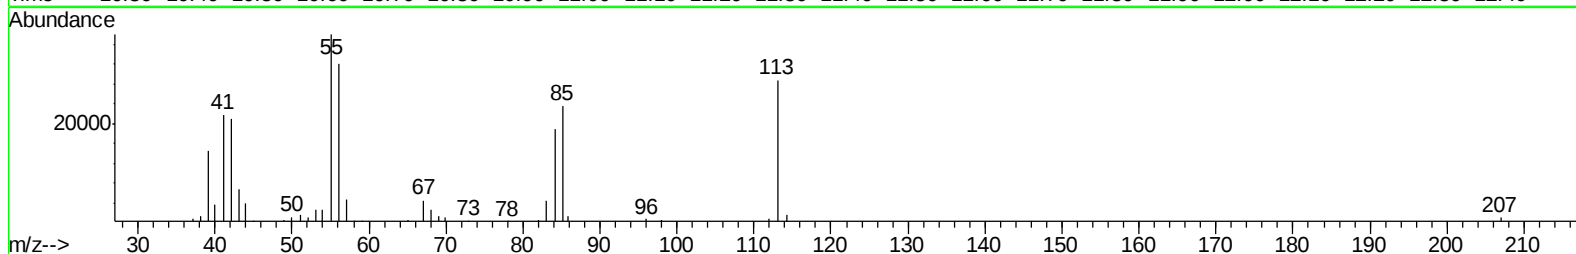


Data File : BM017731.D
Acq On : 21 Nov 2018 07:42
Operator : MJ/SJ
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Nov 21 08:15:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 21 07:44:17 2018
Response via : Initial Calibration

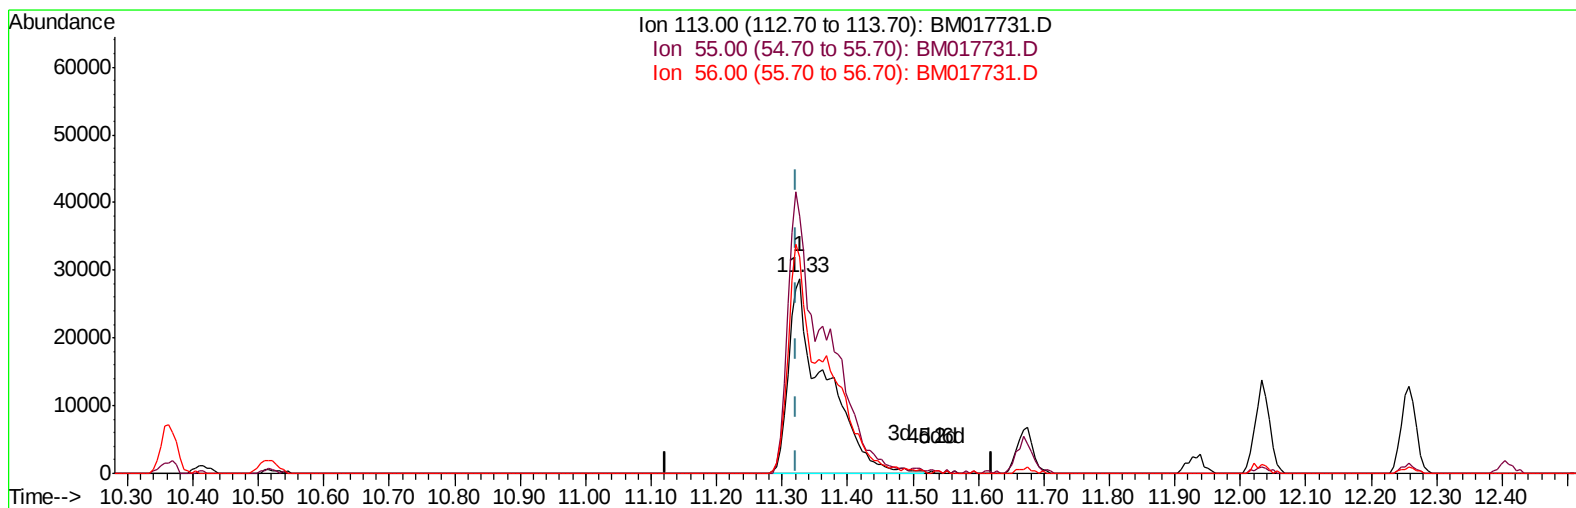

TIC: BM017731.D

(32) Caprolactam

11.328min (+0.006) 19.68ng/ul m

response 110324

Ion	Exp%	Act%
113.00	100	100
55.00	138.30	131.99
56.00	110.30	111.18
0.00	0.00	0.00