

Data File : BM017729.D
Acq On : 21 Nov 2018 06:30
Operator : MJ/SJ
Sample : J5990-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETO77

Quant Time: Nov 21 07:47:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 21 07:44:17 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	225482	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1029045	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	646420	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	1486971	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	1437991	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	1208464	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	7879	1.60	ng/uL	0.00
5) Phenol-d5	6.78	99	148930	7.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	348915	28.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	401104	24.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	291728	17.34	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	236948	29.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	269639	29.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	472996	27.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	190	0.01	ng/ul	0.02
43) Dimethylphthalate-d6	13.66	166	1669876	29.77	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	2015954	29.70	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	57843	5.67	ng/ul	0.02
57) Fluorene-d10	15.24	176	1452845	30.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	271054	25.50	ng/ul	0.00
70) Anthracene-d10	17.10	188	2282106	30.83	ng/ul	0.00
78) Pyrene-d10	19.40	212	2488854	35.77	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	2057570	31.39	ng/ul	0.00


Target Compounds					Qvalue
33) 4-Chloro-3-methylphenol	11.72	107	36998	2.001	ng/ul# 20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM017729.D
Acq On : 21 Nov 2018 06:30
Operator : MJ/SJ
Sample : J5990-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETO77

Quant Time: Nov 21 07:47:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 21 07:44:17 2018
Response via : Initial Calibration

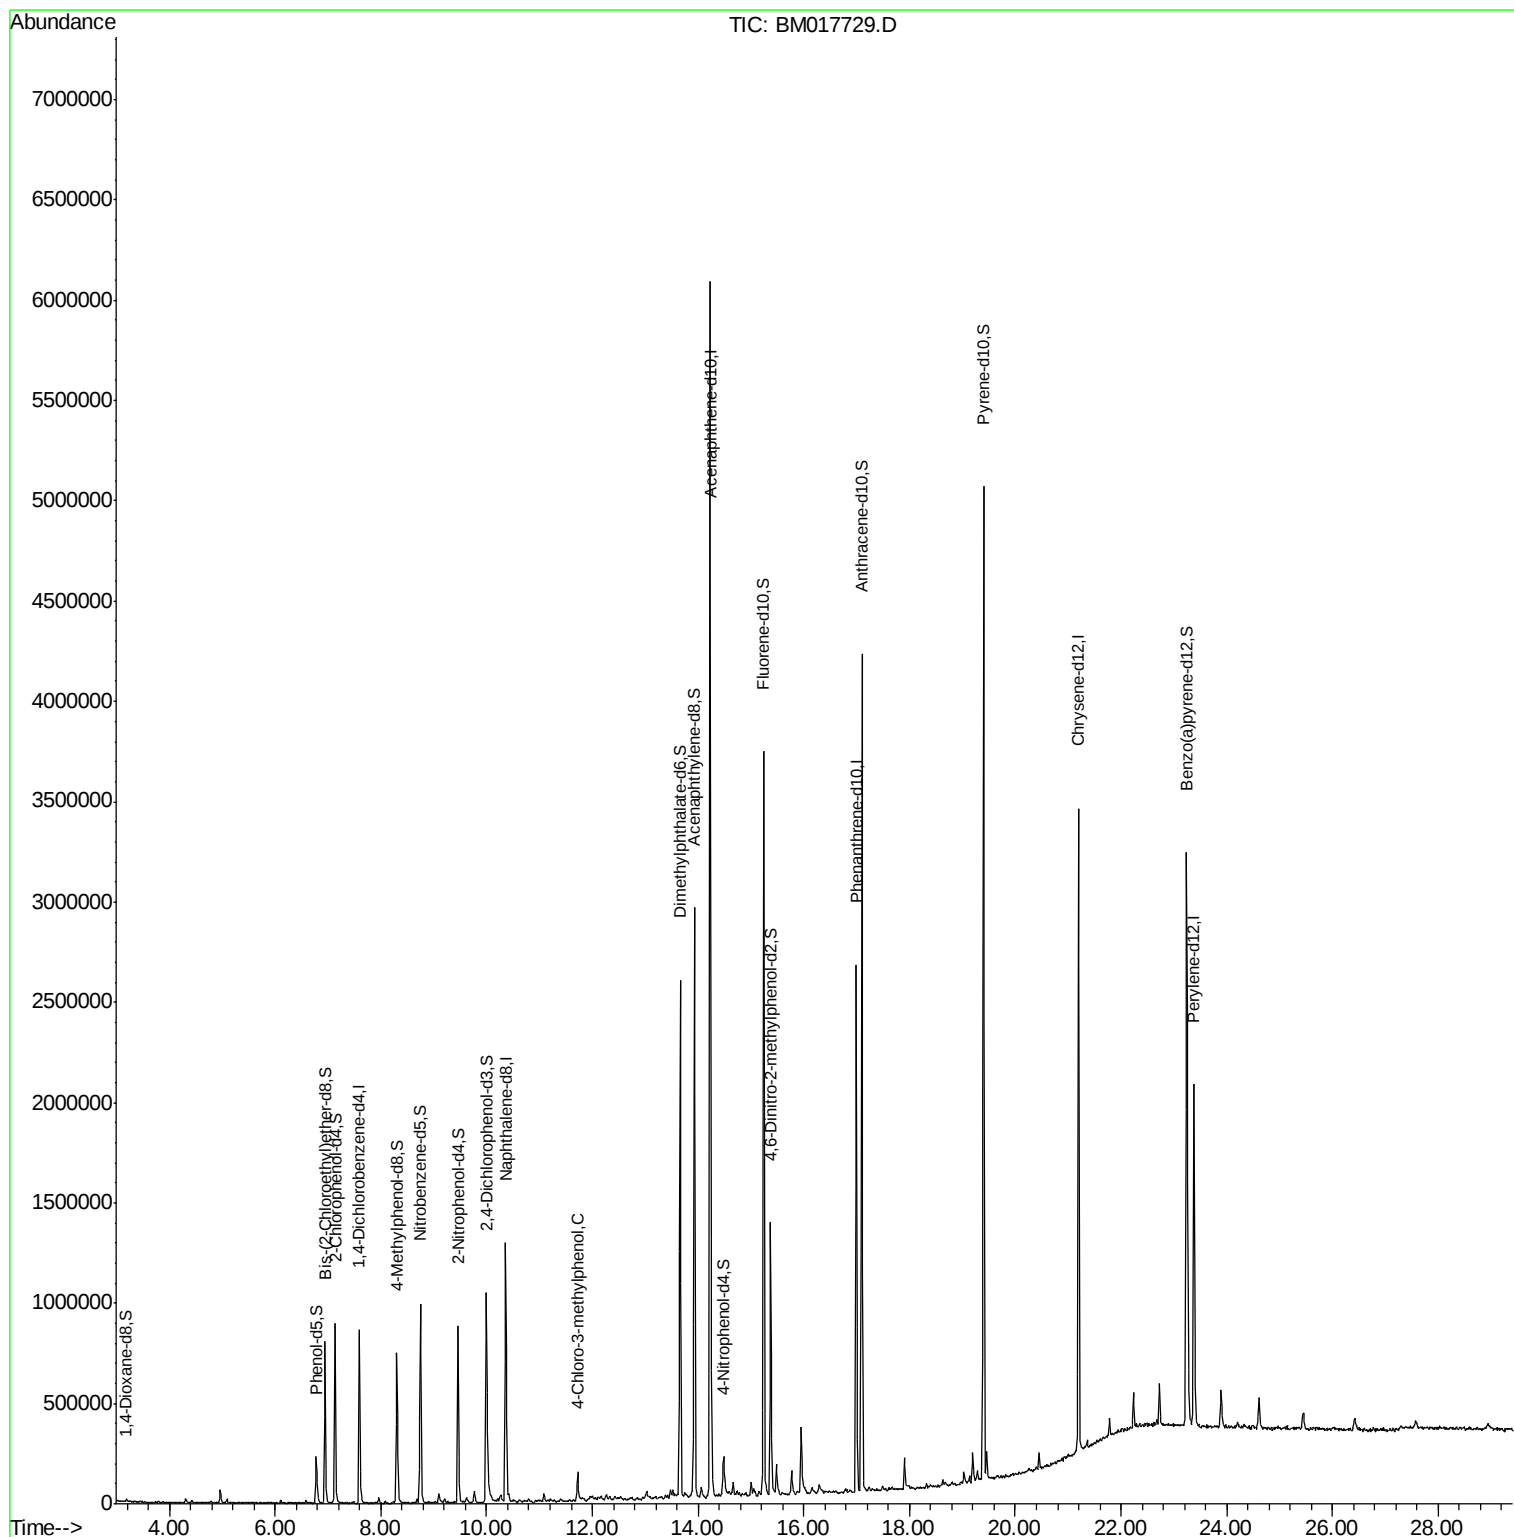

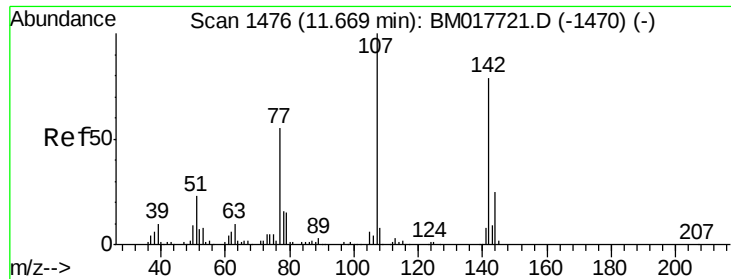

#33

4-Chloro-3-methylphenol

Concen: 2.001 ng/ul

RT: 11.72 min Scan# 1485

Delta R.T. 0.05 min

Lab File: BM017729.D

Acq: 21 Nov 2018 06:30

Instrument :

BNA_M

ClientSampleId :

ETO77


Tgt Ion:107 Resp: 36998

Ion Ratio Lower Upper

107 100

144 0.0 21.1 31.7#

142 0.0 63.0 94.6#

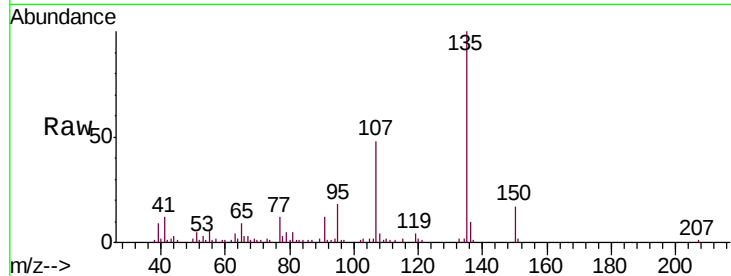

Abundance

Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E

