

Data File : BM017730.D
Acq On : 21 Nov 2018 07:06
Operator : MJ/SJ
Sample : J5990-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETO79

Quant Time: Nov 21 07:47:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 21 07:44:17 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	247636	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1136442	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	706766	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	1630236	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	1765818	20.00	ng/ul	0.00
85) Perylene-d12	23.39	264	1501421	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.19	96	25593	4.73	ng/uL	0.00
5) Phenol-d5	6.78	99	177002	7.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	422332	30.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	478883	27.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	328265	17.76	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	284705	32.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	332979	33.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	562817	29.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	17489	1.07	ng/ul	0.02
43) Dimethylphthalate-d6	13.66	166	1972645	32.17	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	2407325	32.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	74224	6.66	ng/ul	0.01
57) Fluorene-d10	15.24	176	1707988	32.25	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	347680	29.83	ng/ul	0.00
70) Anthracene-d10	17.10	188	2748729	33.87	ng/ul	0.00
78) Pyrene-d10	19.40	212	3158251	36.96	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.25	264	2863841	35.17	ng/ul	0.00


Target Compounds				Qvalue		
33) 4-Chloro-3-methylphenol	11.72	107	43264	2.119	ng/ul#	20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM017730.D
Acq On : 21 Nov 2018 07:06
Operator : MJ/SJ
Sample : J5990-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETO79

Quant Time: Nov 21 07:47:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 21 07:44:17 2018
Response via : Initial Calibration

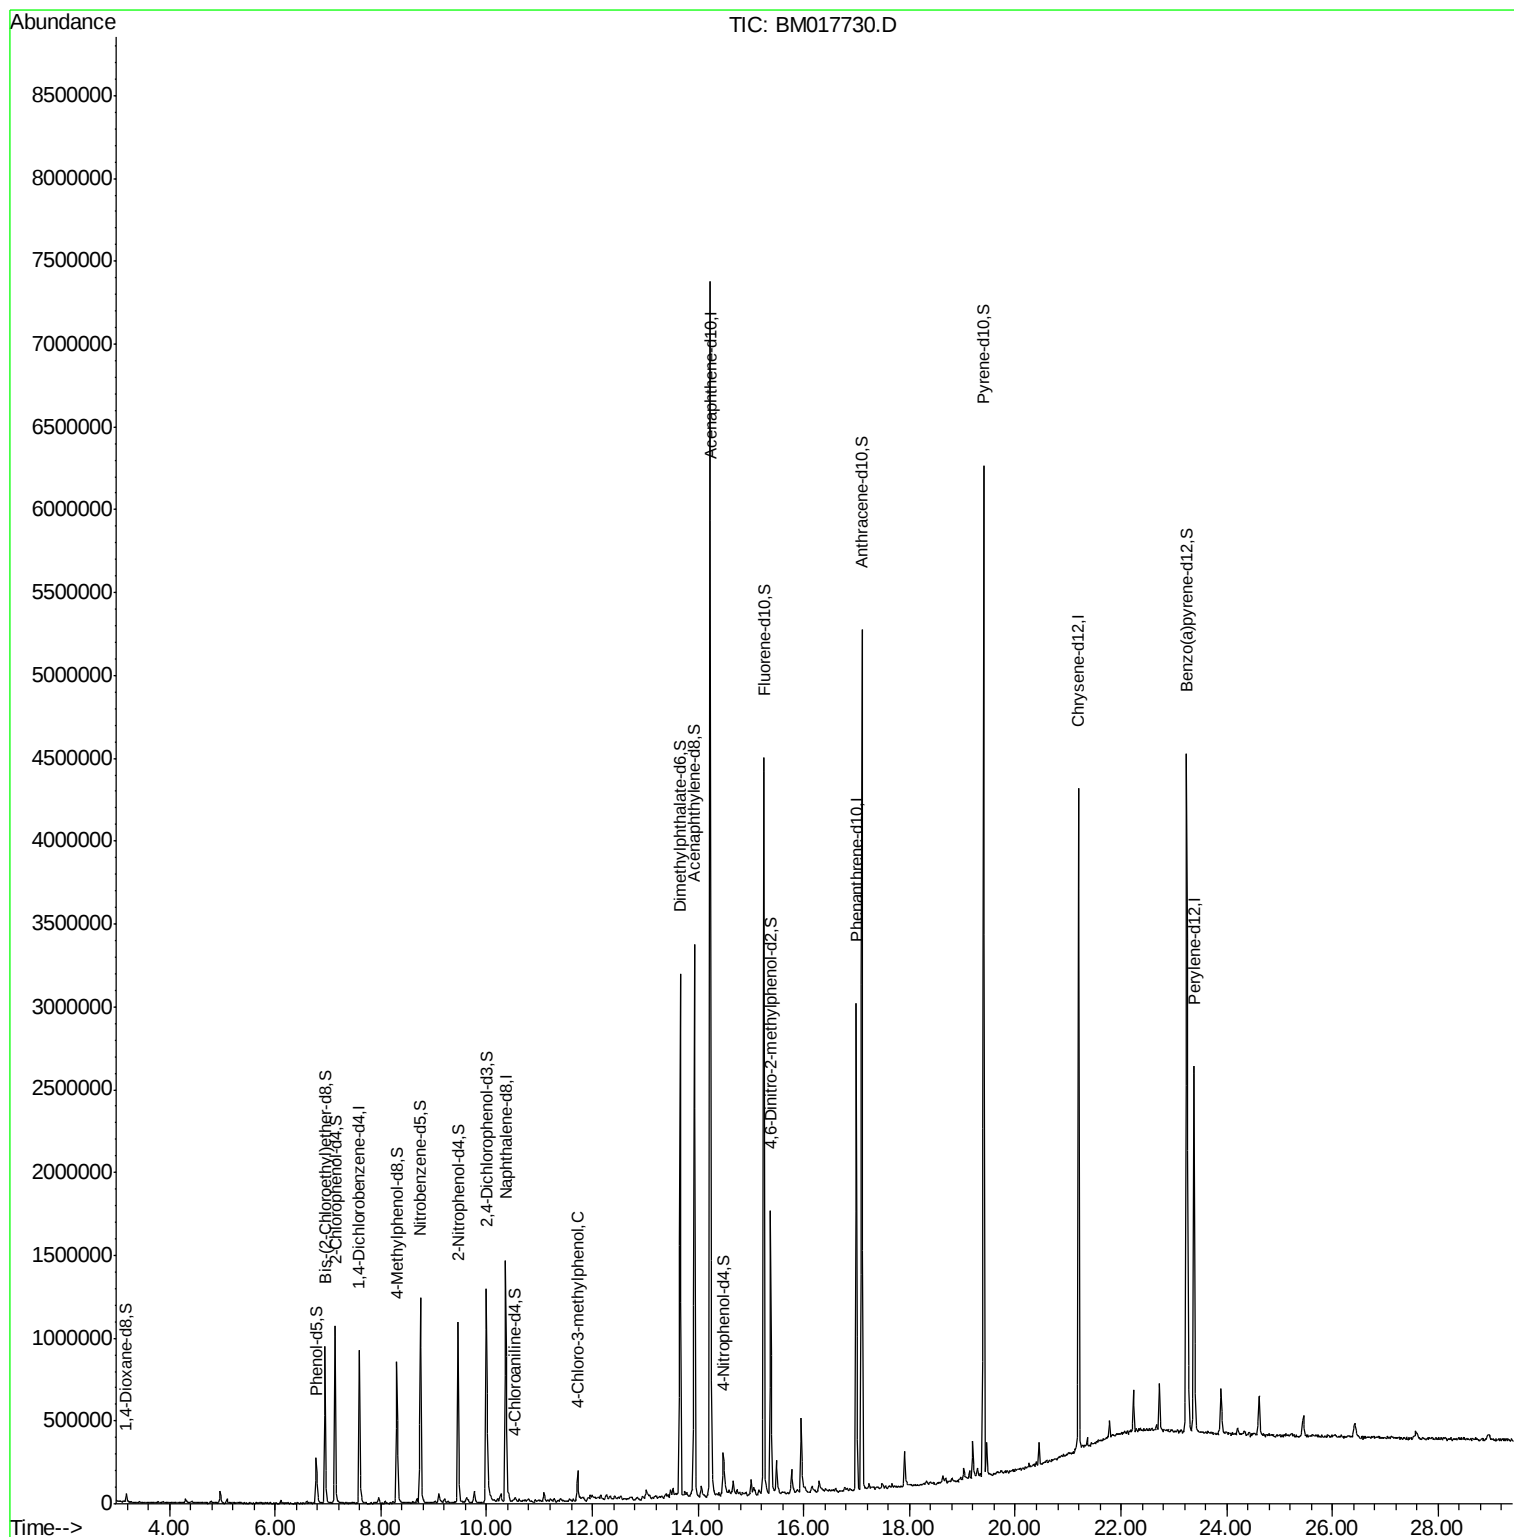

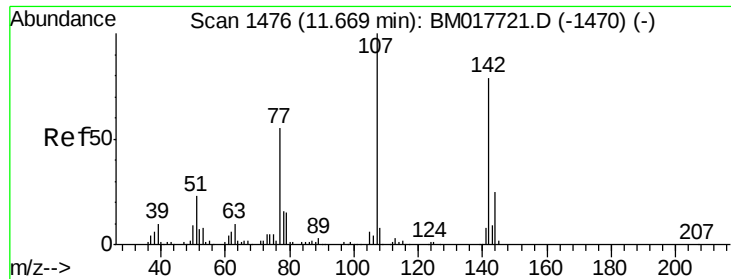

#33

4-Chloro-3-methylphenol

Concen: 2.119 ng/ul

RT: 11.72 min Scan# 1485

Delta R.T. 0.05 min

Lab File: BM017730.D

Acq: 21 Nov 2018 07:06

Instrument :

BNA_M

ClientSampleId :

ETO79


Tgt Ion:107 Resp: 43264

Ion Ratio Lower Upper

107 100

144 0.0 21.1 31.7#

142 0.0 63.0 94.6#

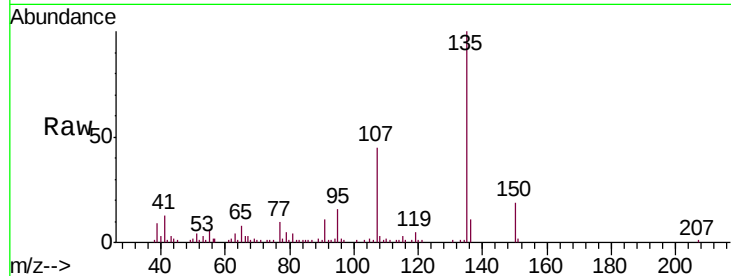

Abundance Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E

