

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
 Data File : BM042922.D
 Acq On : 20 Nov 2023 11:30
 Operator : MA/JU
 Sample : PB156867BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK867

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	36	rVB2	10899	13104	1.66%	0.169%
2	3.604	102	105	122	rBV	110407	197246	25.00%	2.546%
3	4.469	251	252	256	rVB2	1698	1167	0.15%	0.015%
4	5.575	438	440	442	rVB2	981	927	0.12%	0.012%
5	5.657	451	454	458	rVB5	1141	1550	0.20%	0.020%
6	6.181	542	543	547	rBV2	1780	1589	0.20%	0.021%
7	6.422	582	584	587	rVB4	945	954	0.12%	0.012%
8	6.493	594	596	600	rVB4	1100	1565	0.20%	0.020%
9	6.522	600	601	604	rBV3	913	995	0.13%	0.013%
10	6.975	673	678	695	rBV	116360	230253	29.18%	2.972%
11	7.157	704	709	721	rBV	102284	174707	22.14%	2.255%
12	7.328	733	738	751	rBV	131669	236985	30.03%	3.059%
13	7.463	759	761	764	rVV3	1034	1061	0.13%	0.014%
14	7.492	764	766	774	rVB4	1555	2315	0.29%	0.030%
15	7.710	802	803	807	rVB3	879	951	0.12%	0.012%
16	7.810	814	820	836	rBV	100888	185991	23.57%	2.401%
17	8.116	870	872	875	rBV2	921	1031	0.13%	0.013%
18	8.328	904	908	910	rBV3	647	824	0.10%	0.011%
19	8.534	936	943	961	rBV	117654	251925	31.93%	3.252%
20	8.728	974	976	979	rVB4	1061	1165	0.15%	0.015%
21	9.010	1018	1024	1043	rBV	111999	222598	28.21%	2.873%
22	9.351	1080	1082	1085	rVB3	1294	1182	0.15%	0.015%
23	9.428	1093	1095	1097	rVV3	1070	932	0.12%	0.012%
24	9.451	1097	1099	1102	rVB3	1084	1040	0.13%	0.013%
25	9.722	1140	1145	1160	rBV	95764	191665	24.29%	2.474%
26	9.839	1164	1165	1167	rVV2	1322	829	0.11%	0.011%
27	9.998	1189	1192	1193	rVB2	967	931	0.12%	0.012%
28	10.075	1203	1205	1209	rBV5	829	998	0.13%	0.013%
29	10.251	1229	1235	1251	rBV2	103473	231142	29.29%	2.984%
30	10.622	1291	1298	1310	rBV	131879	231261	29.31%	2.985%
31	10.804	1322	1329	1343	rBV	84179	217808	27.60%	2.812%
32	11.222	1398	1400	1402	rVB2	1177	834	0.11%	0.011%
33	11.263	1404	1407	1410	rVB3	765	963	0.12%	0.012%
34	12.010	1532	1534	1537	rBV2	808	901	0.11%	0.012%
35	12.257	1573	1576	1580	rBV4	1116	1352	0.17%	0.017%
36	12.698	1649	1651	1656	rBV2	723	1278	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
 Data File : BM042922.D
 Acq On : 20 Nov 2023 11:30
 Operator : MA/JU
 Sample : PB156867BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK867

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	12.780	1660	1665	1666	rVV4	507	813	0.10%	0.010%
38	13.269	1744	1748	1751	rVB3	596	896	0.11%	0.012%
39	13.316	1751	1756	1761	rBV	1899	2929	0.37%	0.038%
40	13.892	1848	1854	1870	rBV	260237	401882	50.93%	5.188%
41	13.992	1870	1871	1875	rVB3	1084	1085	0.14%	0.014%
42	14.074	1882	1885	1890	rVB4	668	1295	0.16%	0.017%
43	14.163	1894	1900	1911	rVV	265660	413501	52.40%	5.338%
44	14.251	1914	1915	1918	rVB2	1337	1165	0.15%	0.015%
45	14.463	1945	1951	1964	rBV	189207	288533	36.56%	3.725%
46	14.745	1992	1999	2013	rBV4	24785	99193	12.57%	1.280%
47	14.980	2037	2039	2041	rVB2	1282	832	0.11%	0.011%
48	15.068	2049	2054	2057	rVB4	730	1085	0.14%	0.014%
49	15.463	2115	2121	2135	rVV	339764	527182	66.81%	6.805%
50	15.610	2142	2146	2160	rBV	96506	172476	21.86%	2.226%
51	15.698	2160	2161	2164	rVB3	2464	1577	0.20%	0.020%
52	16.139	2234	2236	2242	rVB2	675	803	0.10%	0.010%
53	16.286	2256	2261	2263	rVB2	584	804	0.10%	0.010%
54	16.333	2267	2269	2272	rBV2	761	827	0.10%	0.011%
55	16.886	2360	2363	2366	rVB3	779	1098	0.14%	0.014%
56	17.221	2414	2420	2431	rBV	230251	344878	43.71%	4.452%
57	17.321	2431	2437	2458	rVV	365676	584430	74.06%	7.544%
58	17.486	2461	2465	2470	rVB4	945	2111	0.27%	0.027%
59	17.827	2522	2523	2528	rVB3	983	1015	0.13%	0.013%
60	18.074	2561	2565	2576	rBV6	11707	30459	3.86%	0.393%
61	18.239	2591	2593	2596	rVB2	996	1091	0.14%	0.014%
62	18.374	2614	2616	2619	rBV3	835	912	0.12%	0.012%
63	18.445	2625	2628	2631	rBV4	964	1241	0.16%	0.016%
64	18.551	2643	2646	2647	rVB2	1019	808	0.10%	0.010%
65	18.615	2656	2657	2660	rBV3	1085	967	0.12%	0.012%
66	18.639	2660	2661	2666	rVB2	976	1280	0.16%	0.017%
67	18.739	2674	2678	2679	rVB2	992	986	0.12%	0.013%
68	18.774	2679	2684	2686	rBV4	1032	1781	0.23%	0.023%
69	18.921	2707	2709	2713	rVB3	1145	1103	0.14%	0.014%
70	18.962	2713	2716	2717	rBV	1160	1049	0.13%	0.014%
71	19.033	2726	2728	2732	rVB3	1375	1282	0.16%	0.017%
72	19.074	2732	2735	2736	rBV2	937	926	0.12%	0.012%
73	19.180	2748	2753	2761	rBV5	4389	7134	0.90%	0.092%
74	19.256	2761	2766	2770	rBV4	4356	6026	0.76%	0.078%
75	19.362	2780	2784	2785	rBV2	6480	6677	0.85%	0.086%
76	19.468	2800	2802	2804	rBV2	1180	895	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
Data File : BM042922.D
Acq On : 20 Nov 2023 11:30
Operator : MA/JU
Sample : PB156867BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK867

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	19.492	2804	2806	2813	rBV7	1319	1678	0.21%	0.022%
78	19.562	2815	2818	2819	rBV3	2293	1987	0.25%	0.026%
79	19.615	2821	2827	2839	rBV	551690	731964	92.76%	9.449%
80	19.956	2883	2885	2887	rBV3	1528	1455	0.18%	0.019%
81	20.309	2943	2945	2947	rBV3	2074	1921	0.24%	0.025%
82	21.409	3127	3132	3142	rBV	254721	411755	52.18%	5.315%
83	23.603	3499	3505	3521	rVB2	405354	789099	100.00%	10.186%
84	23.762	3525	3532	3548	rVB	216814	479724	60.79%	6.193%




Sum of corrected areas: 7746629

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
Data File : BM042922.D
Acq On : 20 Nov 2023 11:30
Operator : MA/JU
Sample : PB156867BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK867

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

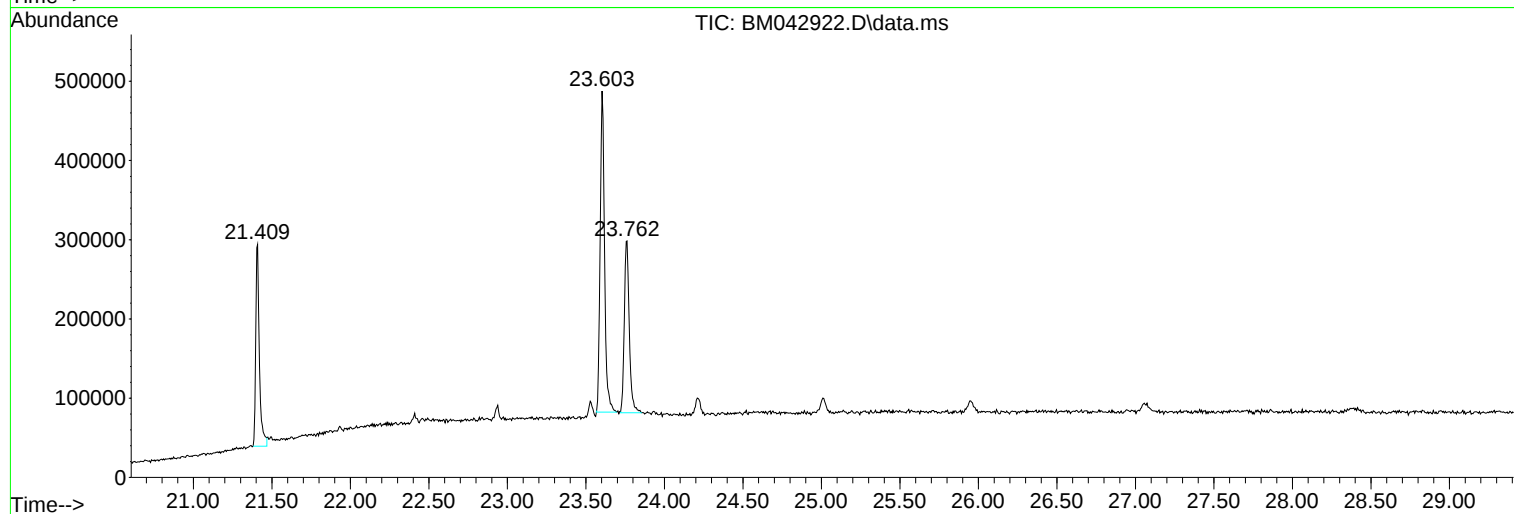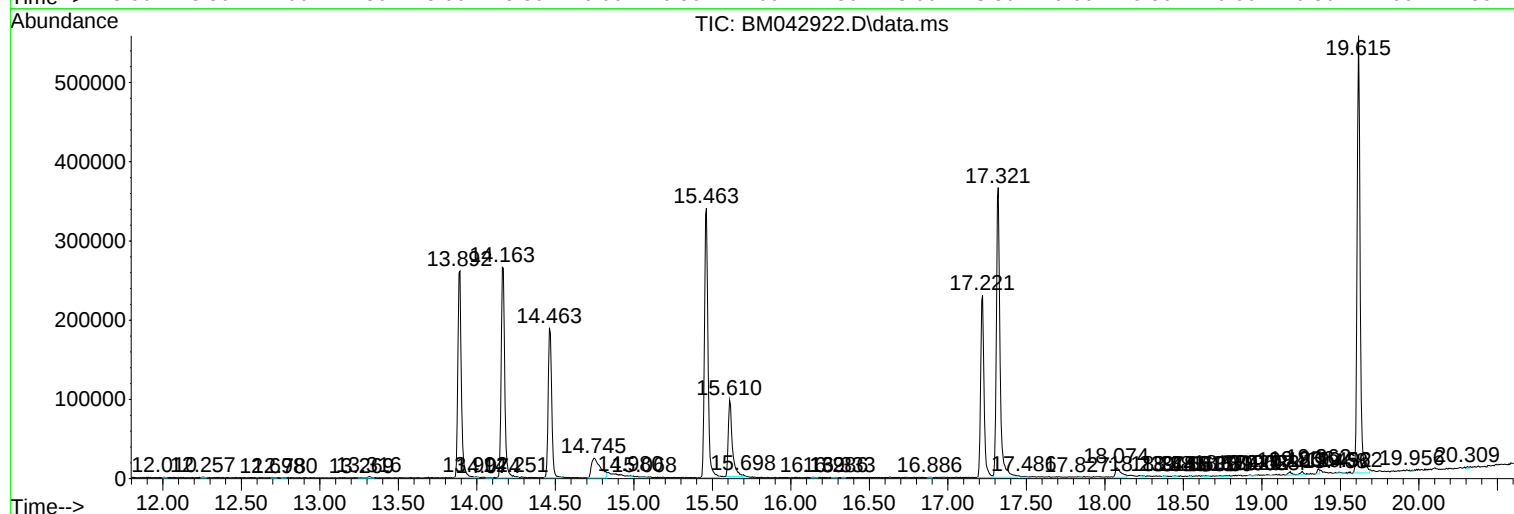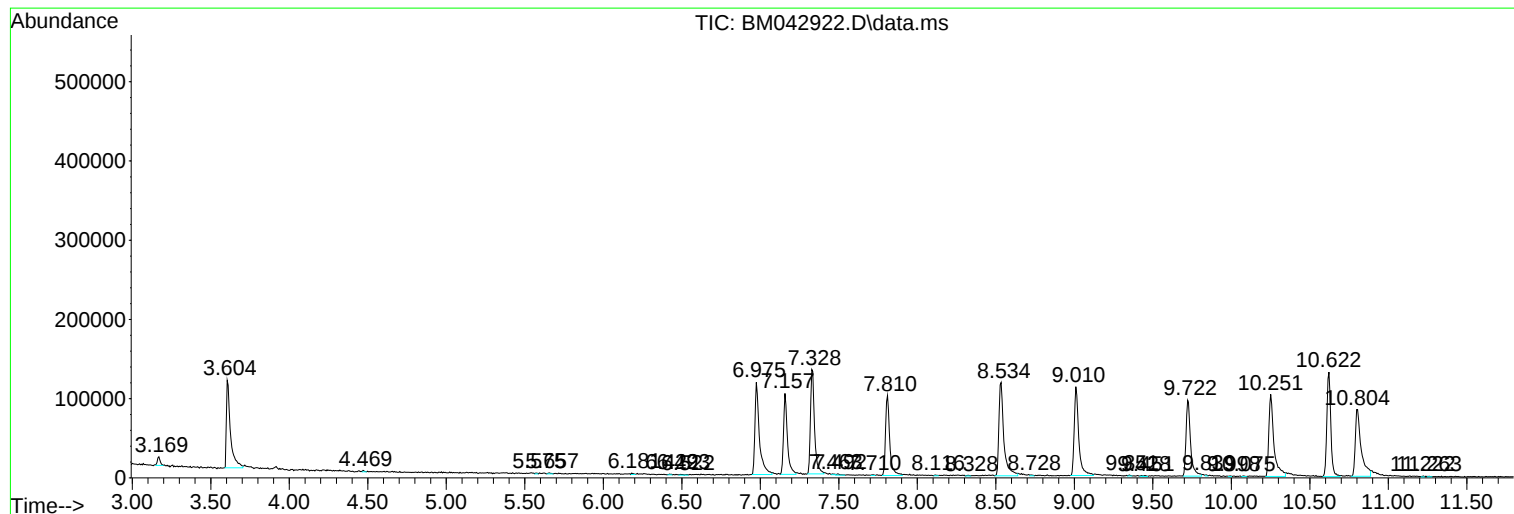

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
Data File : BM042922.D
Acq On : 20 Nov 2023 11:30
Operator : MA/JU
Sample : PB156867BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK867

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
Data File : BM042922.D
Acq On : 20 Nov 2023 11:30
Operator : MA/JU
Sample : PB156867BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK867

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc