

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
 Data File : BM042923.D
 Acq On : 20 Nov 2023 12:06
 Operator : MA/JU
 Sample : PB157217BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	39	rVB	12276	16934	2.01%	0.223%
2	3.604	102	105	125	rBV	117728	203874	24.24%	2.685%
3	4.087	185	187	190	rVB3	1764	1116	0.13%	0.015%
4	4.599	272	274	279	rBV3	1201	1335	0.16%	0.018%
5	4.781	303	305	307	rBV3	1432	1427	0.17%	0.019%
6	5.040	347	349	352	rVB3	1467	1241	0.15%	0.016%
7	5.587	441	442	445	rBV3	875	928	0.11%	0.012%
8	5.734	464	467	468	rBV3	1173	983	0.12%	0.013%
9	6.016	509	515	517	rVB4	876	1037	0.12%	0.014%
10	6.140	534	536	538	rBV2	1094	1008	0.12%	0.013%
11	6.404	578	581	583	rBV4	874	866	0.10%	0.011%
12	6.975	673	678	698	rBV	119657	242588	28.85%	3.194%
13	7.157	704	709	723	rBV	100573	171535	20.40%	2.259%
14	7.328	732	738	752	rBV	138714	248629	29.57%	3.274%
15	7.492	764	766	771	rVB4	1461	1255	0.15%	0.017%
16	7.810	814	820	835	rBV	83235	150768	17.93%	1.985%
17	8.204	884	887	889	rBV3	976	1082	0.13%	0.014%
18	8.528	937	942	958	rBV	122091	248708	29.58%	3.275%
19	8.704	970	972	974	rVB2	1117	980	0.12%	0.013%
20	8.898	1001	1005	1006	rBV2	1019	1179	0.14%	0.016%
21	9.010	1018	1024	1041	rBV	117840	227392	27.04%	2.994%
22	9.722	1139	1145	1159	rBV	100137	193923	23.06%	2.554%
23	9.904	1174	1176	1182	rBV5	730	988	0.12%	0.013%
24	9.975	1184	1188	1193	rVB4	901	968	0.12%	0.013%
25	10.251	1229	1235	1254	rBV	108128	244007	29.02%	3.213%
26	10.369	1254	1255	1264	rVB5	2868	5360	0.64%	0.071%
27	10.622	1289	1298	1311	rBV	107293	192810	22.93%	2.539%
28	10.798	1323	1328	1356	rBV2	85255	241174	28.68%	3.176%
29	11.086	1375	1377	1380	rVV2	1028	1306	0.16%	0.017%
30	11.128	1380	1384	1387	rVB3	1012	1360	0.16%	0.018%
31	11.298	1411	1413	1416	rBV3	796	842	0.10%	0.011%
32	11.580	1455	1461	1462	rBV4	704	1064	0.13%	0.014%
33	11.933	1517	1521	1522	rVB2	784	862	0.10%	0.011%
34	13.316	1753	1756	1762	rVB3	2363	3618	0.43%	0.048%
35	13.886	1848	1853	1869	rVV	270700	413702	49.20%	5.448%
36	13.992	1869	1871	1873	rVV2	1331	1312	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
 Data File : BM042923.D
 Acq On : 20 Nov 2023 12:06
 Operator : MA/JU
 Sample : PB157217BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.016	1873	1875	1878	rVV3	946	1175	0.14%	0.015%
38	14.063	1880	1883	1887	rBV3	715	1144	0.14%	0.015%
39	14.163	1894	1900	1912	rBV	283200	429906	51.12%	5.661%
40	14.463	1945	1951	1961	rBV	161180	243775	28.99%	3.210%
41	14.739	1992	1998	2012	rBV5	24893	98462	11.71%	1.297%
42	14.863	2017	2019	2022	rVB3	1986	2304	0.27%	0.030%
43	14.980	2037	2039	2043	rVB3	1234	1587	0.19%	0.021%
44	15.045	2049	2050	2052	rBV3	884	909	0.11%	0.012%
45	15.092	2056	2058	2060	rVV	1041	1025	0.12%	0.013%
46	15.139	2064	2066	2069	rVB2	991	1025	0.12%	0.013%
47	15.280	2088	2090	2093	rVB	656	879	0.10%	0.012%
48	15.463	2114	2121	2137	rBV	365537	546014	64.93%	7.190%
49	15.610	2141	2146	2159	rBV	96357	171028	20.34%	2.252%
50	15.757	2170	2171	2177	rVB2	950	1145	0.14%	0.015%
51	17.221	2414	2420	2431	rVV	196717	289052	34.37%	3.806%
52	17.321	2431	2437	2454	rVV	390005	588597	70.00%	7.750%
53	17.433	2454	2456	2461	rVB5	1578	2215	0.26%	0.029%
54	17.533	2470	2473	2475	rBV3	550	848	0.10%	0.011%
55	17.757	2508	2511	2513	rBV2	715	926	0.11%	0.012%
56	18.039	2556	2559	2561	rBV2	910	859	0.10%	0.011%
57	18.086	2561	2567	2573	rBV5	7580	16524	1.97%	0.218%
58	18.427	2622	2625	2627	rBV3	757	916	0.11%	0.012%
59	18.486	2632	2635	2636	rBV2	951	1030	0.12%	0.014%
60	18.733	2674	2677	2681	rBV3	1043	1153	0.14%	0.015%
61	19.186	2748	2754	2757	rBV6	4191	6721	0.80%	0.089%
62	19.256	2761	2766	2770	rBV5	3825	6487	0.77%	0.085%
63	19.362	2781	2784	2785	rBV3	3655	3263	0.39%	0.043%
64	19.580	2819	2821	2822	rBV2	1056	946	0.11%	0.012%
65	19.615	2822	2827	2841	rVV	565375	745526	88.66%	9.817%
66	20.380	2955	2957	2960	rBV4	2103	2275	0.27%	0.030%
67	21.409	3127	3132	3143	rBV	207342	343063	40.80%	4.517%
68	23.603	3498	3505	3521	rBV	410755	840909	100.00%	11.073%
69	23.756	3525	3531	3547	rVB	184269	414489	49.29%	5.458%




Sum of corrected areas: 7594338

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
Data File : BM042923.D
Acq On : 20 Nov 2023 12:06
Operator : MA/JU
Sample : PB157217BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

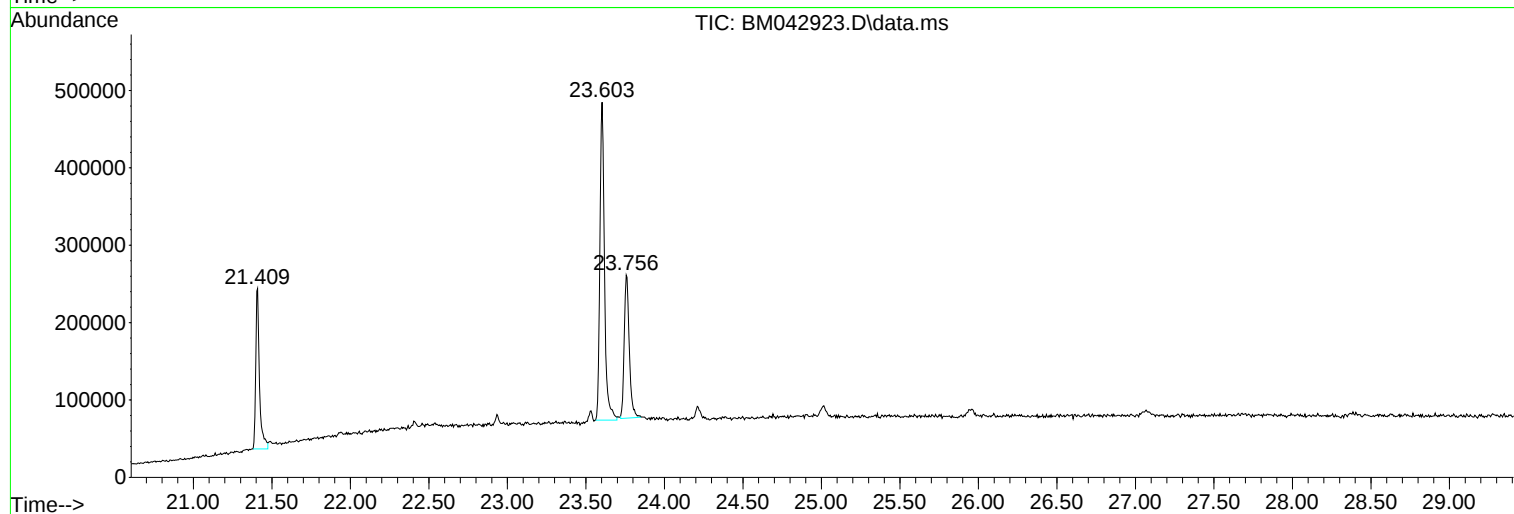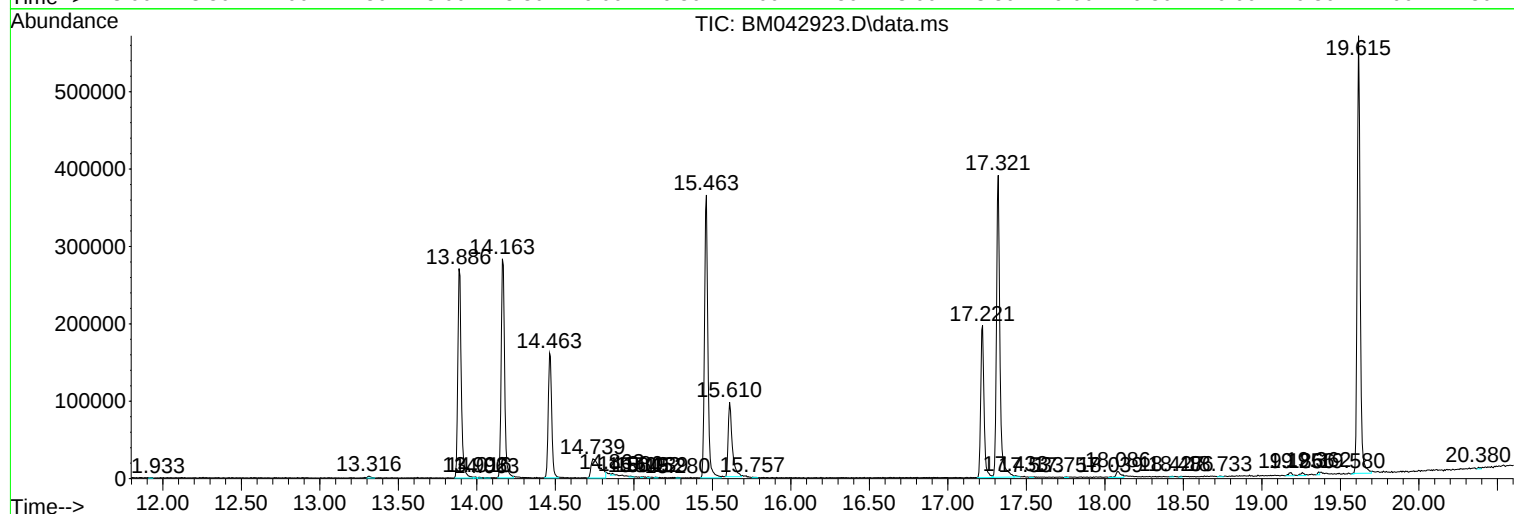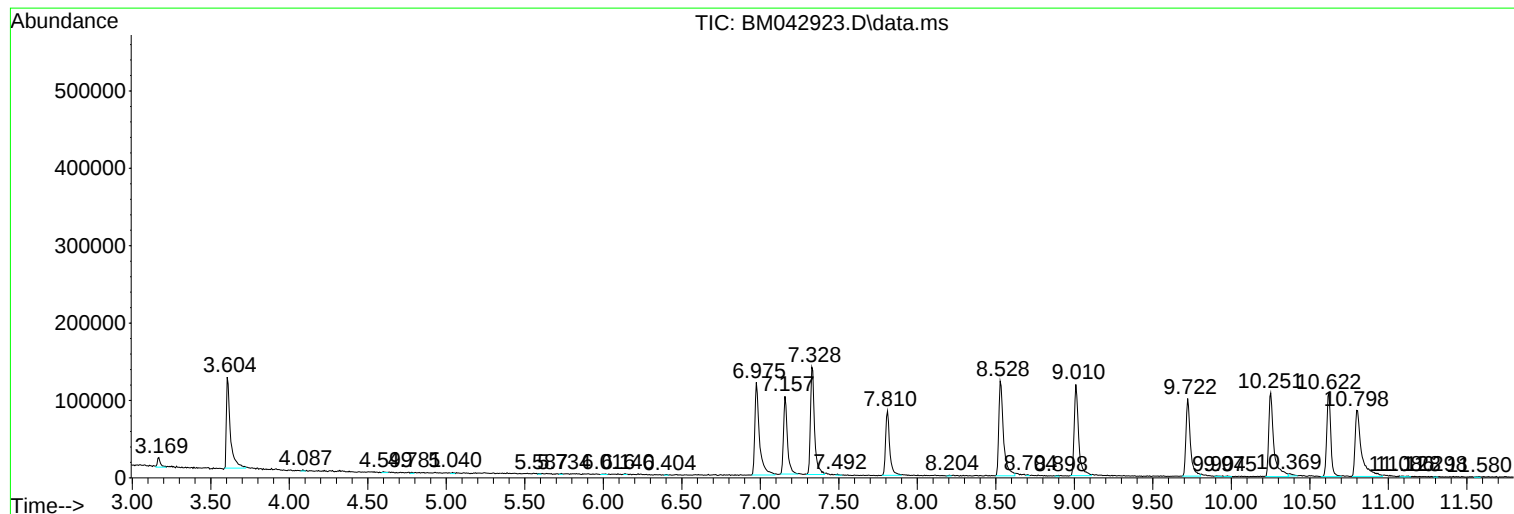

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
Data File : BM042923.D
Acq On : 20 Nov 2023 12:06
Operator : MA/JU
Sample : PB157217BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112023\
Data File : BM042923.D
Acq On : 20 Nov 2023 12:06
Operator : MA/JU
Sample : PB157217BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc