

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112118\
 Data File : BM017742.D
 Acq On : 21 Nov 2018 21:49
 Operator : MJ/SJ
 Sample : J6023-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 111918-TIPC-E-D-B

Quant Time: Nov 22 01:50:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM112118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 12 18:37:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	221317	20.00	ng	-0.02
21) Naphthalene-d8	10.36	136	934705	20.00	ng	-0.02
39) Acenaphthene-d10	14.24	164	601872	20.00	ng	-0.02
64) Phenanthrene-d10	16.99	188	1427291	20.00	ng	-0.02
76) Chrysene-d12	21.20	240	1595233	20.00	ng	-0.02
87) Perylene-d12	23.39	264	1520670	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	422379	32.21	ng	-0.02
7) Phenol-d6	6.78	99	324476	17.72	ng	-0.02
23) Nitrobenzene-d5	8.75	82	1537721	84.93	ng	-0.02
42) 2,4,6-Tribromophenol	15.74	330	719569	83.21	ng	-0.02
45) 2-Fluorobiphenyl	12.86	172	3903762	84.15	ng	-0.02
79) Terphenyl-d14	19.64	244	5512138	78.31	ng	-0.01
Target Compounds						
10) Phenol	6.80	94	61413	3.195	ng	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112118\
Data File : BM017742.D
Acq On : 21 Nov 2018 21:49
Operator : MJ/SJ
Sample : J6023-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
111918-TIPC-E-D-B

Quant Time: Nov 22 01:50:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM112118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

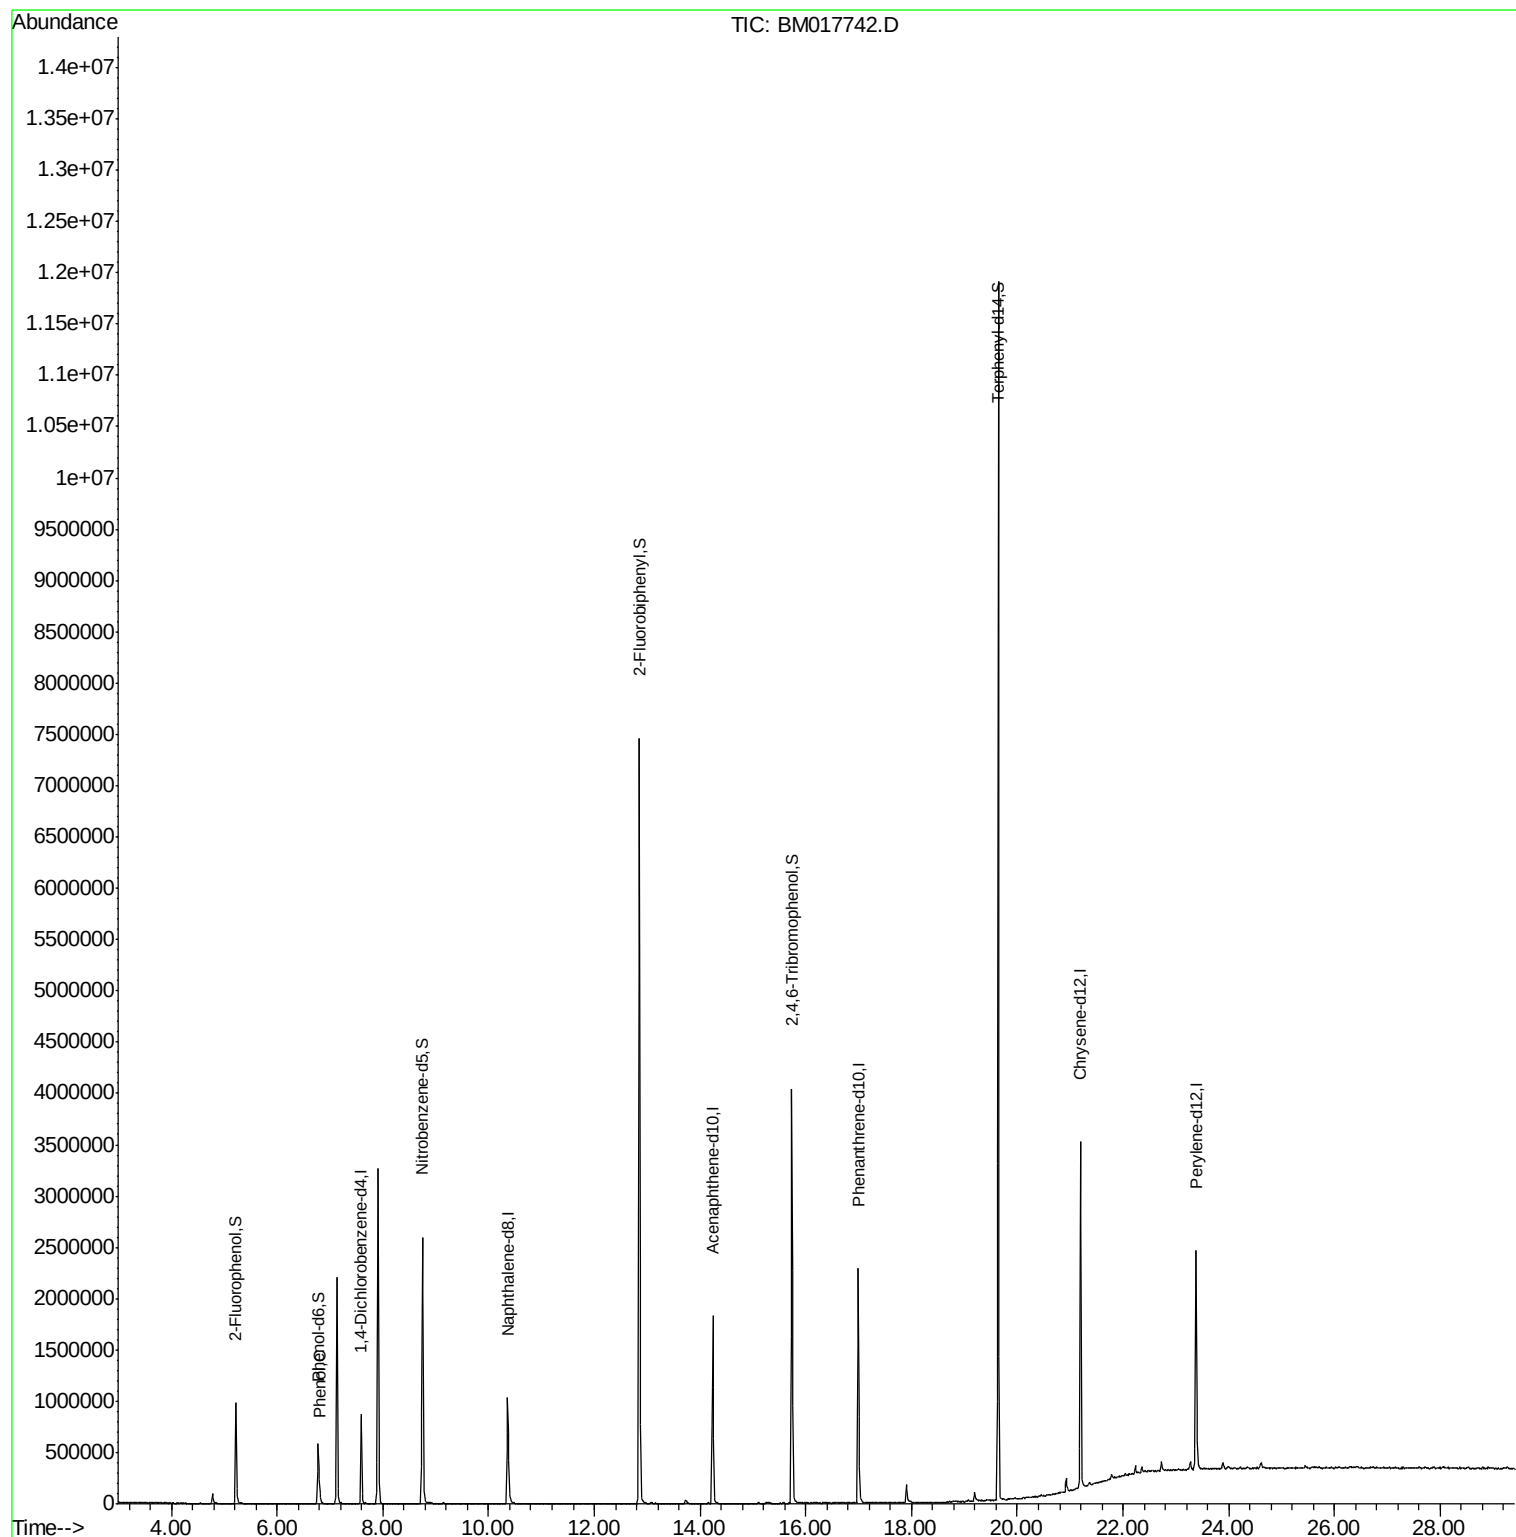

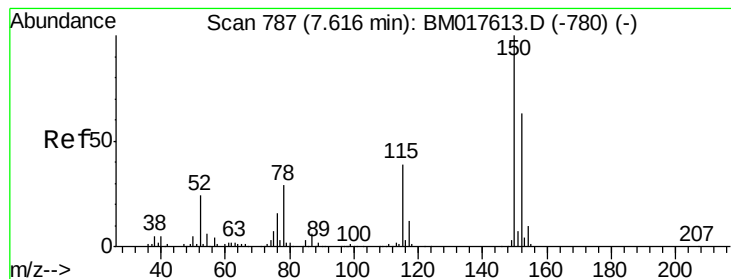

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 7.59 min Scan# 783

Delta R.T. -0.02 min

Lab File: BM017742.D

Acq: 21 Nov 2018 21:49

Instrument :

BNA_M

ClientSampleId :

111918-TIPC-E-D-B


Tgt Ion:152 Resp: 221317

Ion Ratio Lower Upper

152 100

150 150.7 126.4 189.6




115 59.8 49.4 74.0

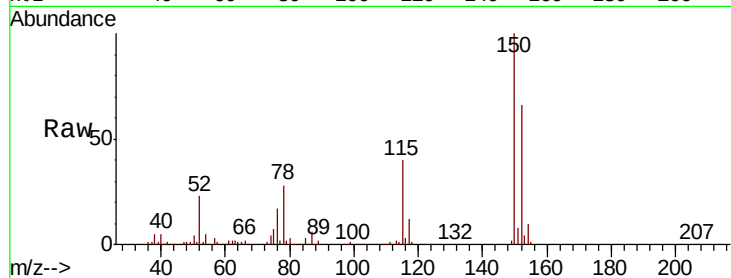

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

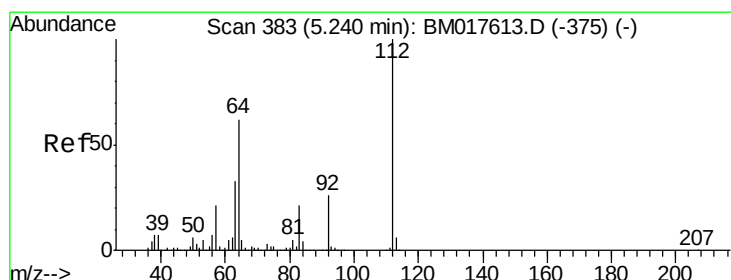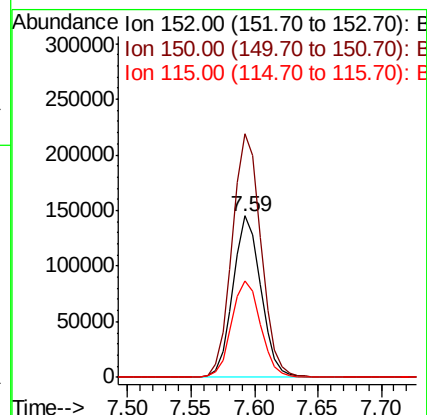

#5

2-Fluorophenol

Concen: 32.208 ng

RT: 5.22 min Scan# 380

Delta R.T. -0.02 min

Lab File: BM017742.D

Acq: 21 Nov 2018 21:49


Tgt Ion:112 Resp: 422379

Ion Ratio Lower Upper

112 100

64 57.6 49.3 73.9



63 32.7 26.2 39.4

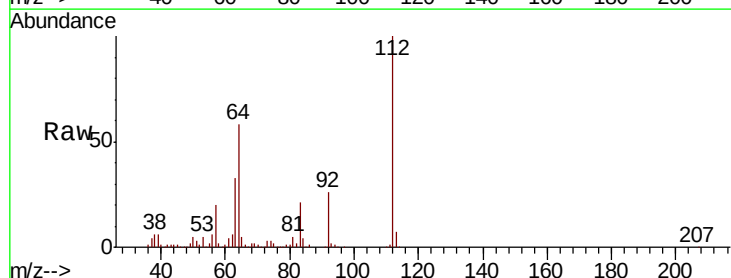


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

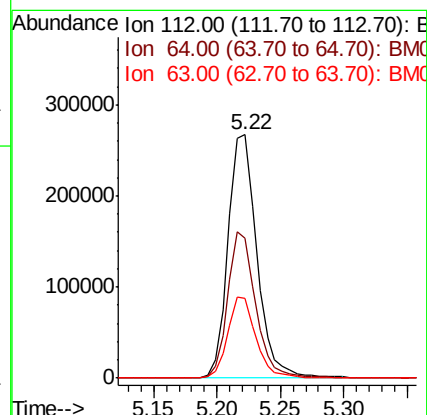



#7

Phenol-d6

Concen: 17.716 ng

RT: 6.78 min Scan# 645

Delta R.T. -0.02 min

Lab File: BM017742.D

Acq: 21 Nov 2018 21:49

Instrument :

BNA_M

ClientSampleId :

111918-TIPC-E-D-B


Tgt Ion: 99 Resp: 324476

Ion Ratio Lower Upper

99 100

42 19.4 16.3 24.5




71 39.2 29.8 44.8

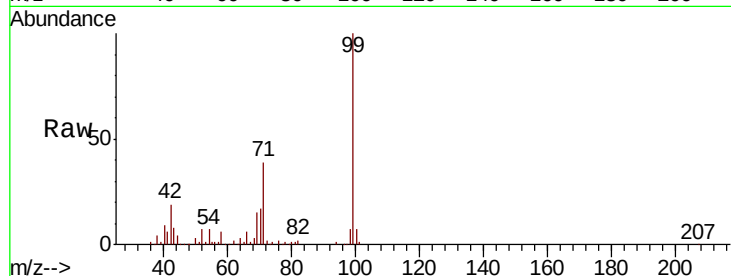

Abundance Ion 99.00 (98.70 to 99.70): BM017742.D (-632) (-)

Ion 42.00 (41.70 to 42.70): BM017742.D (-632) (-)

Ion 71.00 (70.70 to 71.70): BM017742.D (-632) (-)

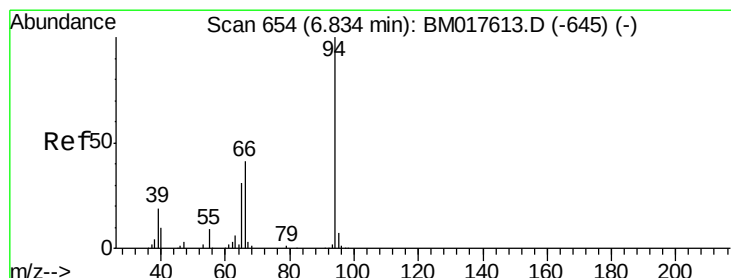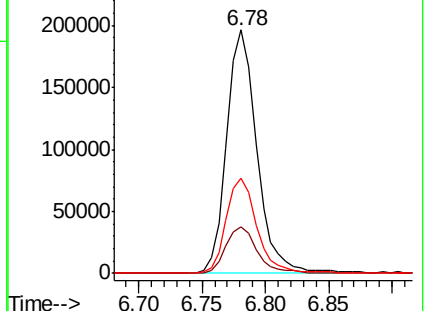

#10

Phenol

Concen: 3.195 ng

RT: 6.80 min Scan# 649

Delta R.T. -0.03 min

Lab File: BM017742.D

Acq: 21 Nov 2018 21:49


Tgt Ion: 94 Resp: 61413

Ion Ratio Lower Upper

94 100

65 29.9 11.4 51.4



66 47.1 21.4 61.4

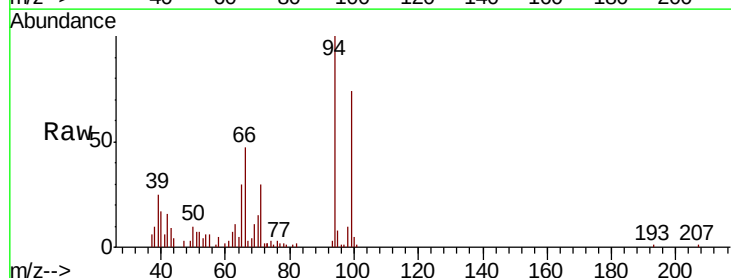


Abundance Ion 94.00 (93.70 to 94.70): BM017742.D (-637) (-)

Ion 65.00 (64.70 to 65.70): BM017742.D (-637) (-)

Ion 66.00 (65.70 to 66.70): BM017742.D (-637) (-)

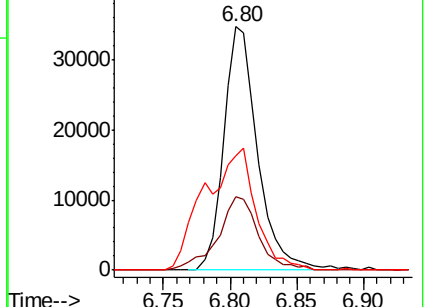


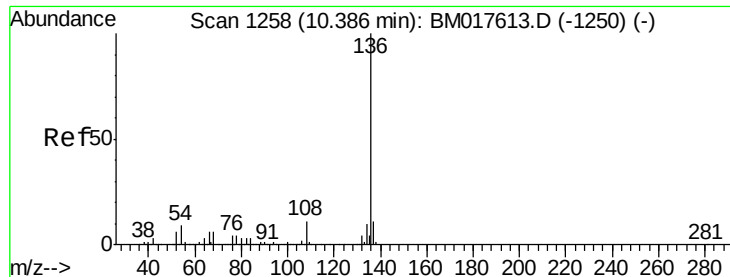




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.36 min Scan# 1254
Delta R.T. -0.02 min
Lab File: BM017742.D
Acq: 21 Nov 2018 21:49

Instrument :
BNA_M
ClientSampleId :
111918-TIPC-E-D-B

Tgt Ion:	136	Resp:	934705
Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.6	12.8
54	7.6	7.0	10.6
68	5.8	4.9	7.3

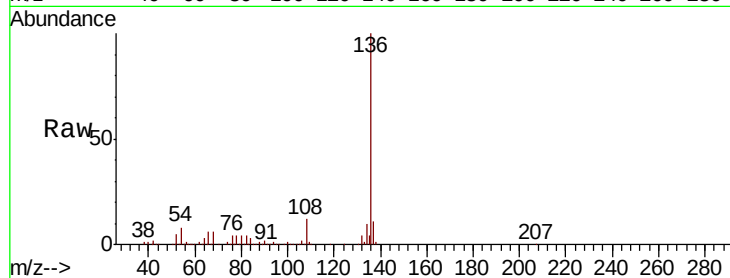


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

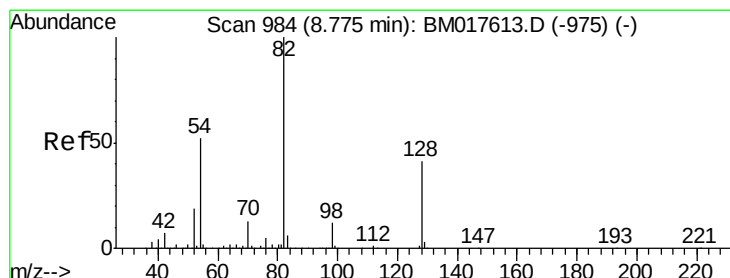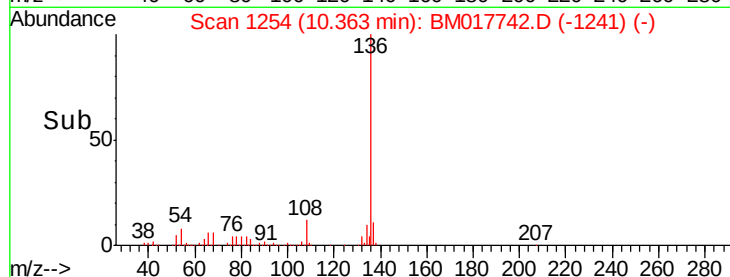
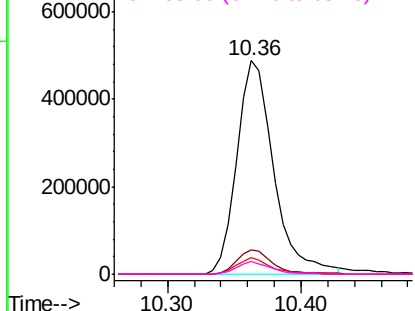



#23
Nitrobenzene-d5
Concen: 84.931 ng
RT: 8.75 min Scan# 980
Delta R.T. -0.02 min
Lab File: BM017742.D
Acq: 21 Nov 2018 21:49

Tgt Ion:	82	Resp:	1537721
Ion	Ratio	Lower	Upper
82	100		
128	41.3	33.0	49.4
54	47.7	41.4	62.2

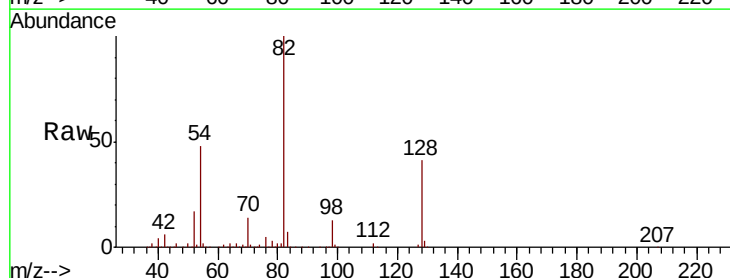

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

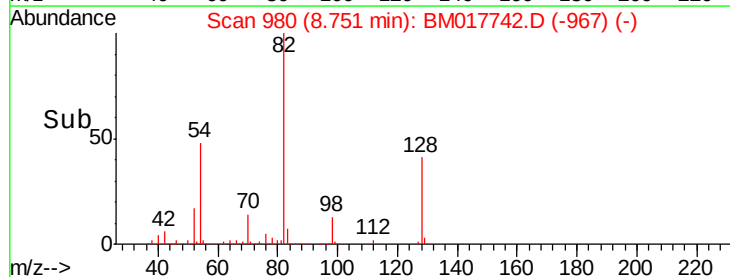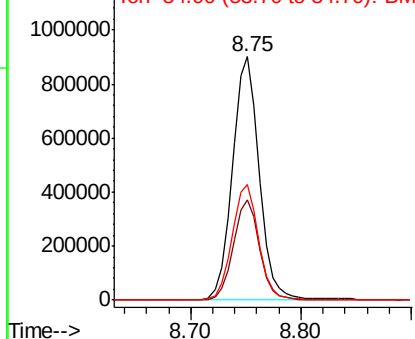

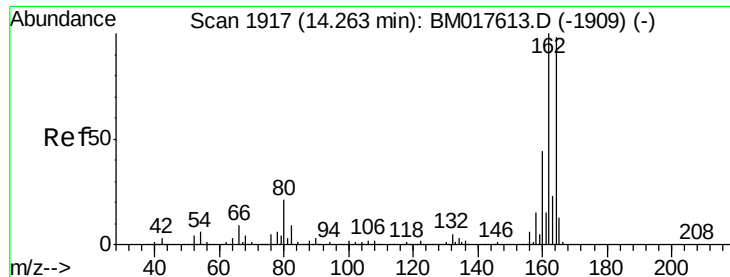

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.24 min Scan# 1913

Delta R.T. -0.02 min

Lab File: BM017742.D

Acq: 21 Nov 2018 21:49

Instrument :

BNA_M

ClientSampleId :

111918-TIPC-E-D-B


Tgt Ion:164 Resp: 601872

Ion Ratio Lower Upper

164 100

162 102.1 81.4 122.0




160 44.8 35.6 53.4

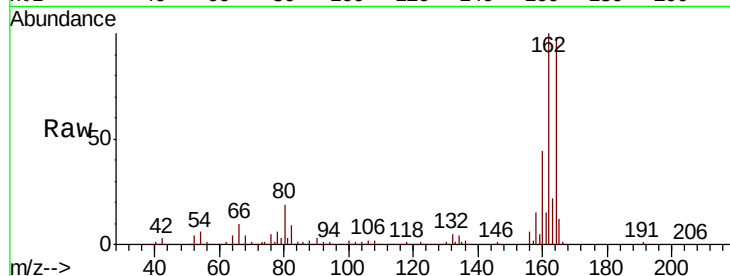

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

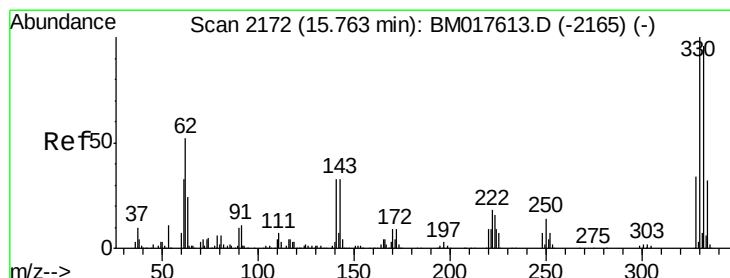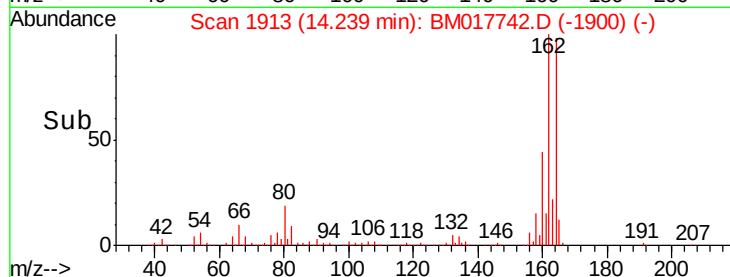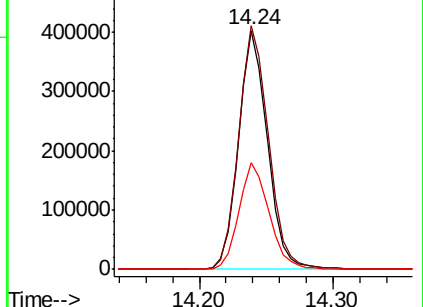

#42

2,4,6-Tribromophenol

Concen: 83.206 ng

RT: 15.74 min Scan# 2168

Delta R.T. -0.02 min

Lab File: BM017742.D

Acq: 21 Nov 2018 21:49


Tgt Ion:330 Resp: 719569

Ion Ratio Lower Upper

330 100

332 96.3 77.9 116.9



141 36.7 27.5 41.3

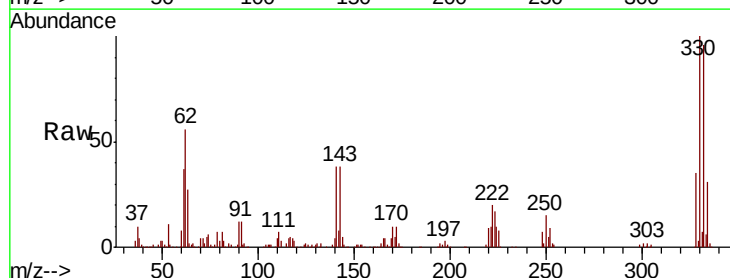


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



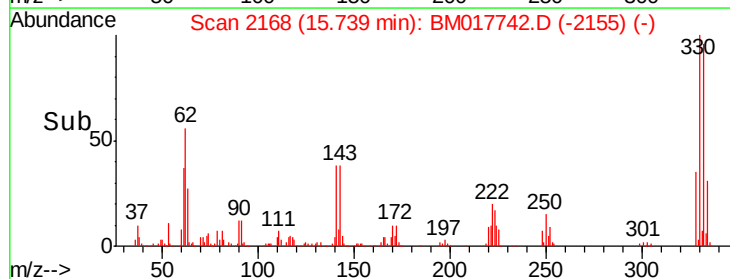
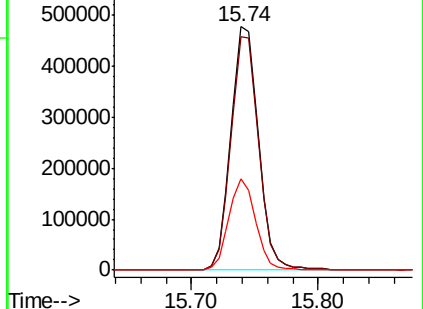




#45
 2-Fluorobiphenyl
 Concen: 84.146 ng
 RT: 12.86 min Scan# 1678
 Delta R.T. -0.02 min
 Lab File: BM017742.D
 Acq: 21 Nov 2018 21:49




Instrument :
 BNA_M
 ClientSampleId :
 111918-TIPC-E-D-B


Tgt Ion:172 Resp: 3903762
 Ion Ratio Lower Upper
 172 100
 171 34.9 28.7 43.1
 170 22.8 18.3 27.5

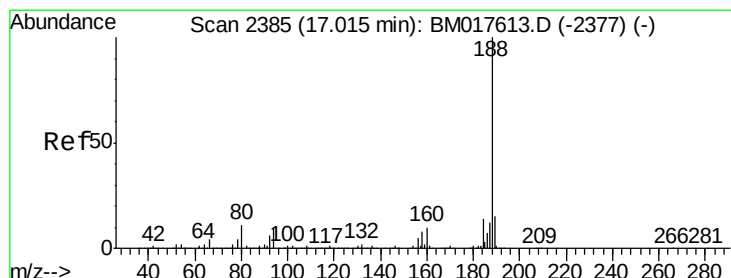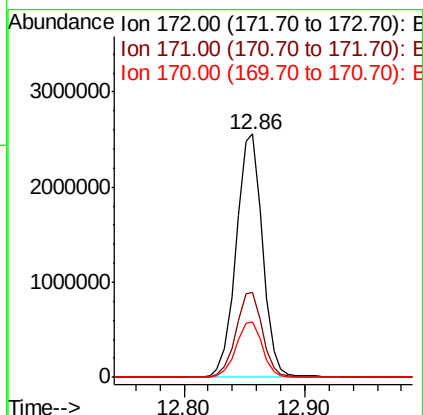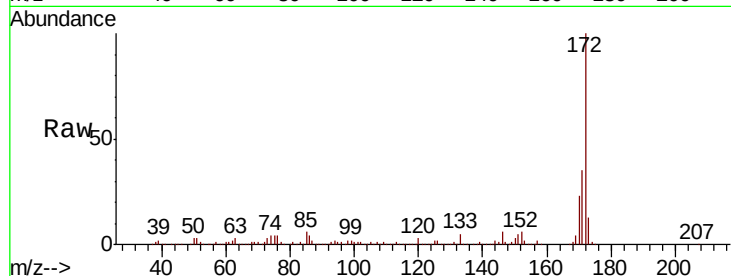

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 16.99 min Scan# 2381
 Delta R.T. -0.02 min
 Lab File: BM017742.D
 Acq: 21 Nov 2018 21:49

Tgt Ion:188 Resp: 1427291
 Ion Ratio Lower Upper
 188 100
 94 9.0 7.5 11.3
 80 10.4 8.6 13.0



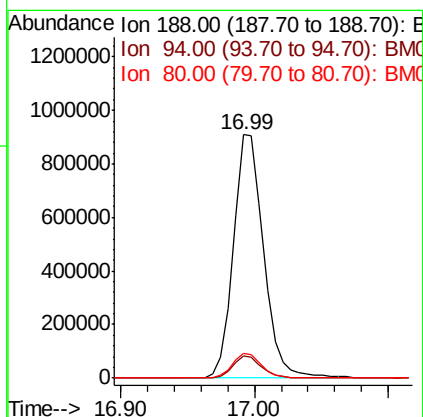
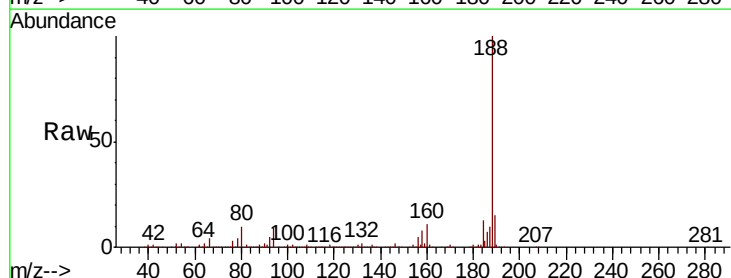




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.20 min Scan# 3096
Delta R.T. -0.02 min
Lab File: BM017742.D
Acq: 21 Nov 2018 21:49




Instrument :
BNA_M
ClientSampleId :
111918-TIPC-E-D-B


Tgt Ion:240 Resp: 1595233
Ion Ratio Lower Upper
240 100
120 9.6 8.5 12.7
236 24.9 20.4 30.6

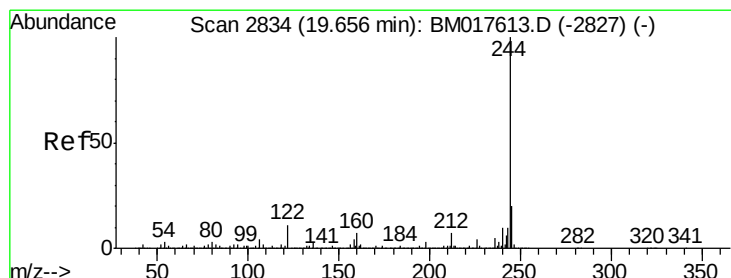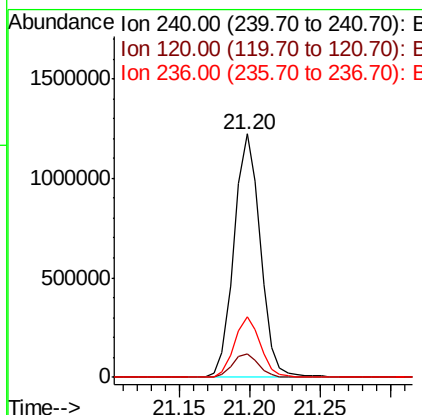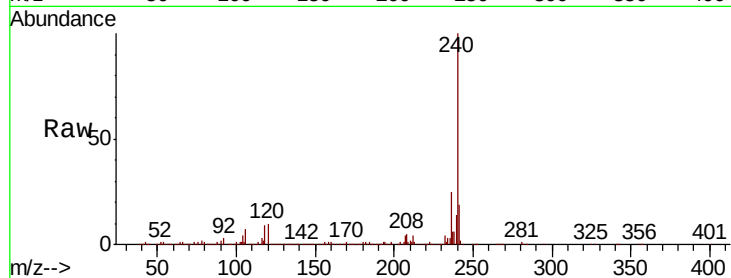

#79
Terphenyl-d14
Concen: 78.313 ng
RT: 19.64 min Scan# 2832
Delta R.T. -0.01 min
Lab File: BM017742.D
Acq: 21 Nov 2018 21:49

Tgt Ion:244 Resp: 5512138
Ion Ratio Lower Upper
244 100
212 7.2 5.8 8.6
122 9.9 9.0 13.6

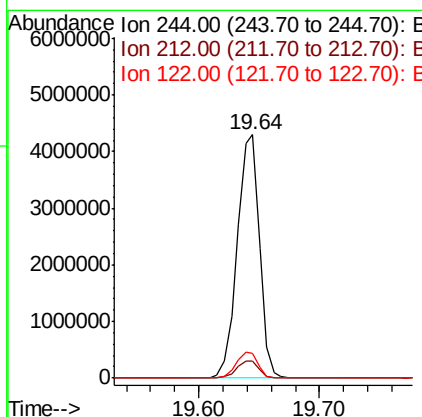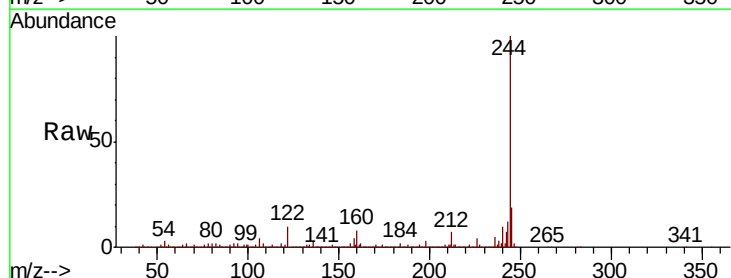

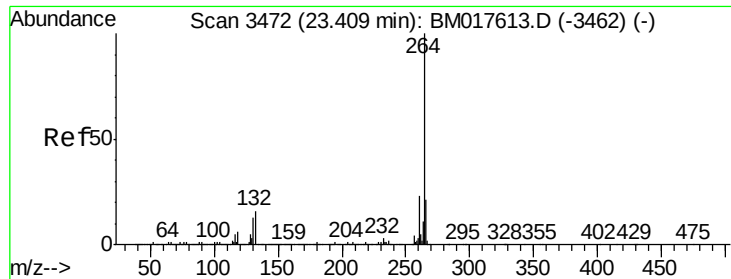

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.39 min Scan# 3468
Delta R.T. -0.02 min
Lab File: BM017742.D
Acq: 21 Nov 2018 21:49

Instrument :
BNA_M
ClientSampleId :
111918-TIPC-E-D-B

Tgt Ion: 264 Resp: 1520670

Ion	Ratio	Lower	Upper
264	100		
260	22.8	18.2	27.2
265	21.5	17.5	26.3

