


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112118\
 Data File : BM017732.D
 Acq On : 21 Nov 2018 15:45
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM112118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

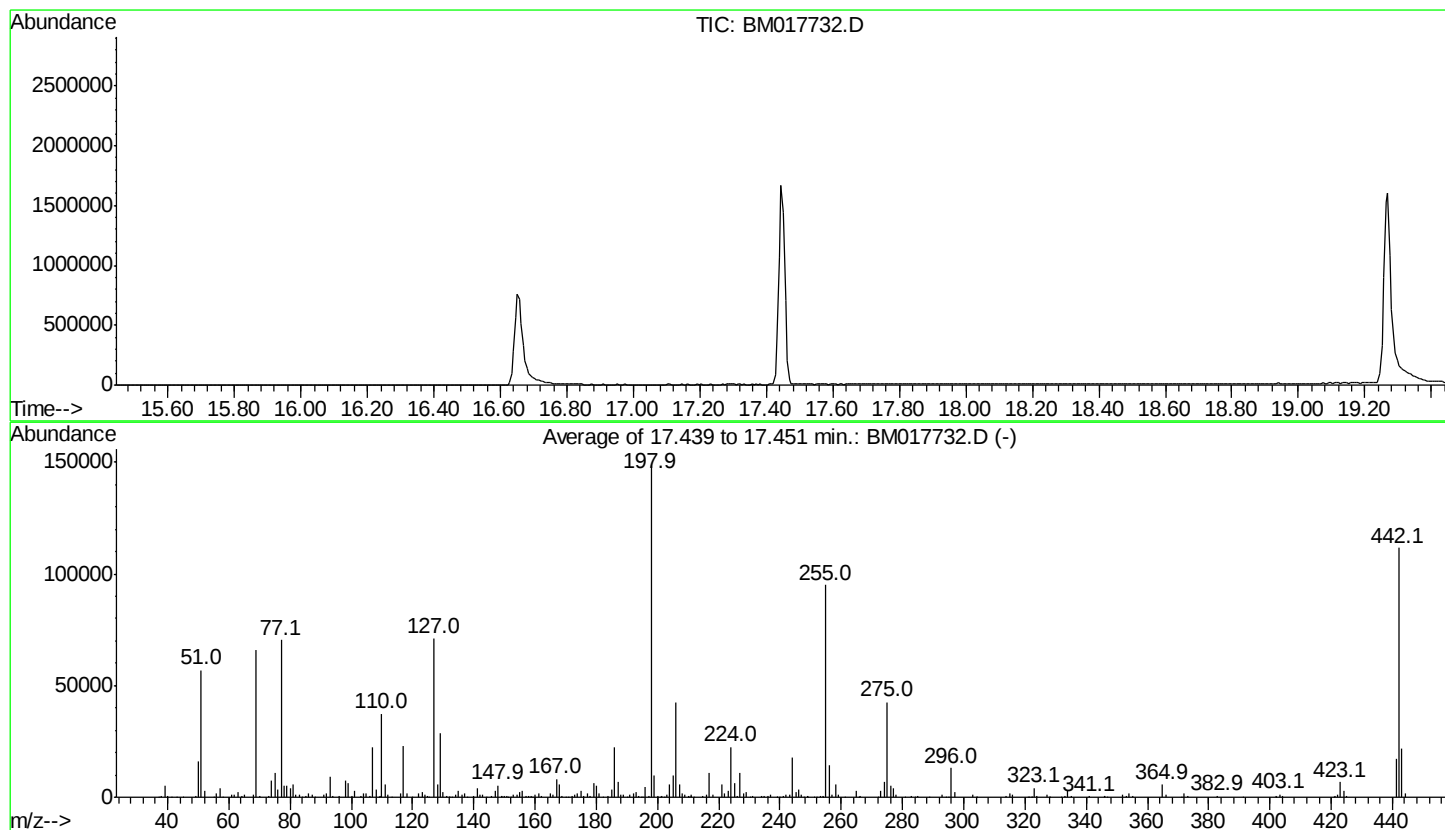

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	56976	PASS
68	69	0.00	2	1.8	1193	PASS
69	198	0.00	100	44.5	66101	PASS
70	69	0.00	2	0.7	480	PASS
127	198	10	80	47.8	70917	PASS
197	198	0.00	2	0.6	870	PASS
198	198	100	100	100.0	148509	PASS
199	198	5	9	6.8	10036	PASS
275	198	10	60	28.7	42608	PASS
365	198	1	100	3.8	5646	PASS
441	198	0.01	100	11.4	17003	PASS
442	198	50	100	75.2	111701	PASS
443	442	15	24	19.7	22018	PASS