

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112119\
 Data File : BM023839.D
 Acq On : 21 Nov 2019 21:07
 Operator : JU
 Sample : K5851-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2

Manual Integrations
 APPROVED

mohammad
 11/22/2019 1:22:51 PM

Quant Time: Nov 22 06:21:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 21 16:09:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	320984	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.29	136	1289212	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.17	164	799358	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.92	188	1727970	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1730389	20.00	ng/ul	0.00
86) Perylene-d12	23.28	264	2136347	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	19489	2.50	ng/uL	0.00
5) Phenol-d5	6.70	99	390945	13.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	226868	13.49	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.05	132	316291	14.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	262094	11.23	ng/ul	-0.01
19) Nitrobenzene-d5	8.66	128	152283	16.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	168400	17.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	306861	13.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	316676	13.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.59	166	967131	15.51	ng/ul	0.00
47) Acenaphthylene-d8	13.86	160	1146275	16.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	97846	9.20	ng/ul	0.00
58) Fluorene-d10	15.17	176	873811	15.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	64242	6.43	ng/ul	0.00
71) Anthracene-d10	17.02	188	1394646	17.01	ng/ul	0.00
79) Pyrene-d10	19.33	212	1660385	18.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.14	264	1970635	17.53	ng/ul	-0.01

Target Compounds

					Ovalue	
45) Dimethylphthalate	13.64	163	342993	5.615	ng/ul	98
70) Phenanthrene	16.96	178	581335	6.108	ng/ul	100
72) Anthracene	17.06	178	124883	1.305	ng/ul	96
77) Fluoranthene	18.99	202	1129692	11.078	ng/ul	96
80) Pyrene	19.36	202	1044188	9.336	ng/ul	98
83) Benzo(a)anthracene	21.12	228	583440	5.112	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	21.07	149	67411	1.260	ng/ul	99
85) Chrysene	21.16	228	608607	5.664	ng/ul	97
88) Benzo(b)fluoranthene	22.64	252	794618	5.835	ng/ul#	97
89) Benzo(k)fluoranthene	22.68	252	306714m	2.338	ng/ul	
91) Benzo(a)pyrene	23.19	252	589419	4.728	ng/ul#	94
92) Indeno(1,2,3-cd)pyrene	25.41	276	445425	3.341	ng/ul	98
93) Dibenzo(a,h)anthracene	25.42	278	120808	1.074	ng/ul#	85
94) Benzo(g,h,i)perylene	26.07	276	452463	4.188	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112119\
Data File : BM023839.D
Acq On : 21 Nov 2019 21:07
Operator : JU
Sample : K5851-14
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AB2

Quant Time: Nov 22 06:21:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 21 16:09:32 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
11/22/2019 1:22:51 PM

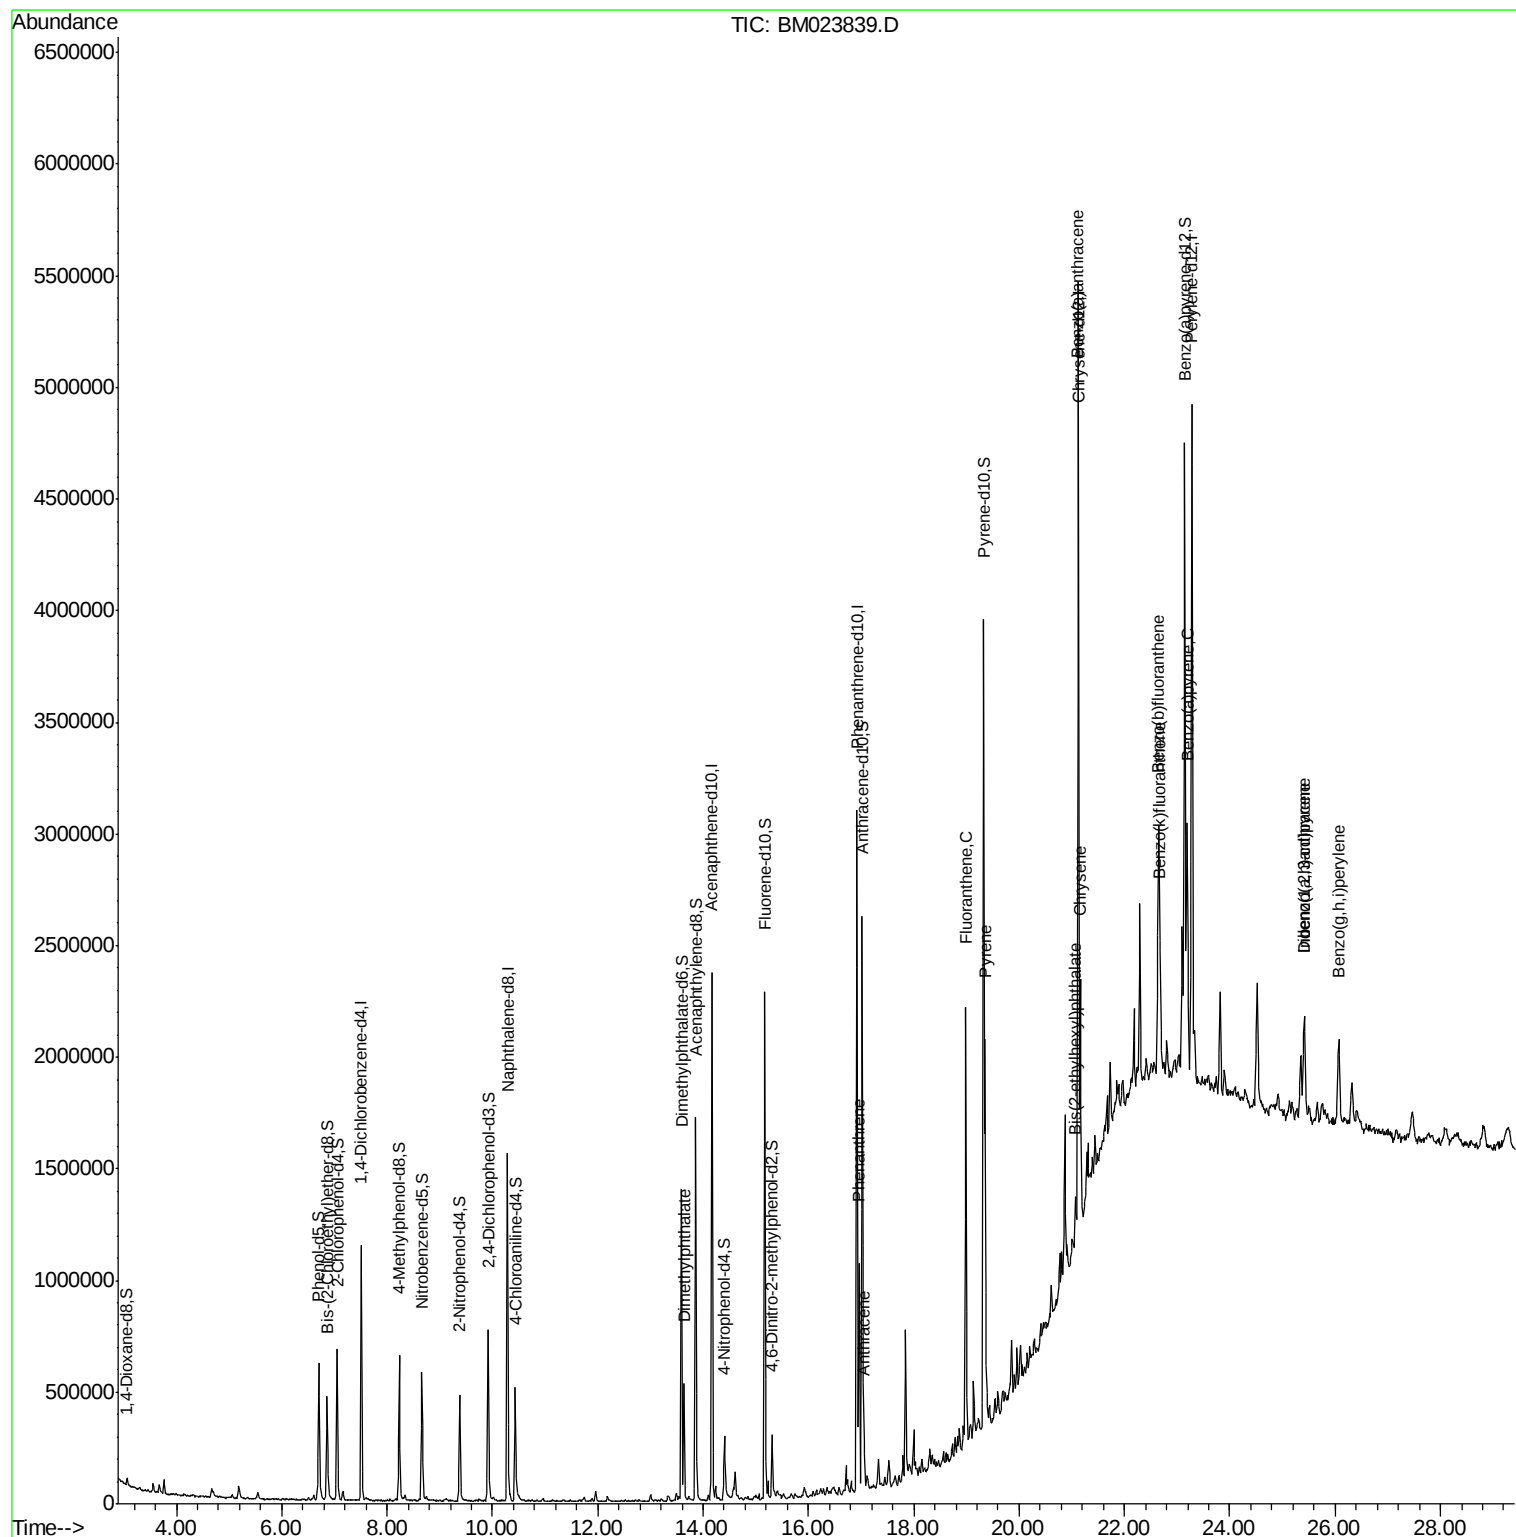

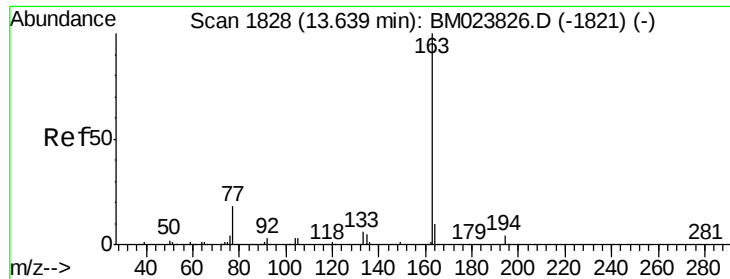





#45
Dimethylphthalate
Concen: 5.615 ng/ul
RT: 13.64 min Scan# 1828
Delta R.T. -0.01 min
Lab File: BM023839.D
Acq: 21 Nov 2019 21:07

Instrument :
BNA_M
ClientSampleId :
C0AB2

Tot Ion	Ratio	Resp	Lower	Upper
163	100	342993		
194	4.0		3.4	5.2
164	9.3		8.0	12.0




Manual Integrations
APPROVED


mohammad
11/22/2019 1:22:51 PM

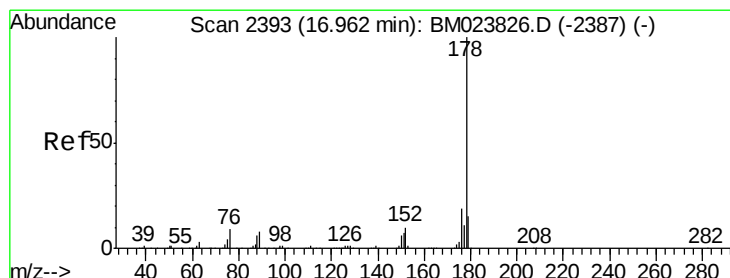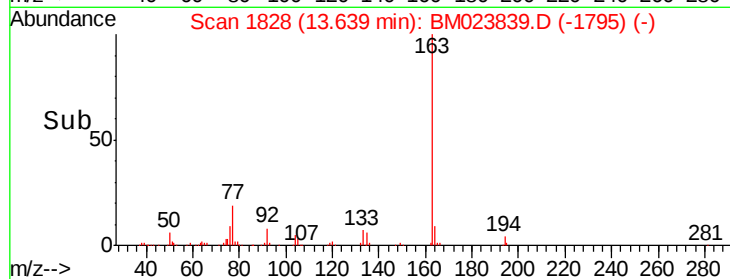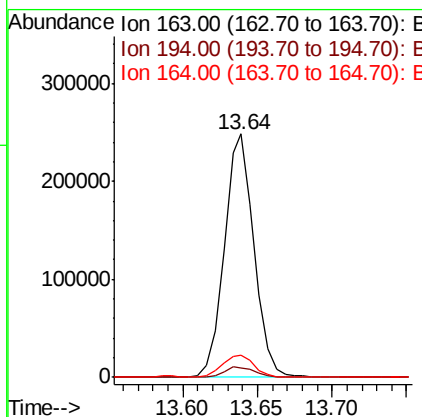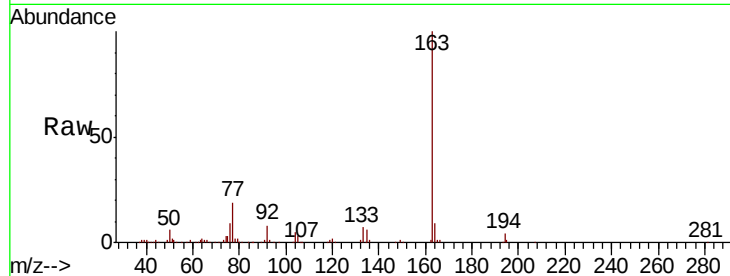

#70
Phenanthrene
Concen: 6.108 ng/ul
RT: 16.96 min Scan# 2393
Delta R.T. -0.01 min
Lab File: BM023839.D
Acq: 21 Nov 2019 21:07

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	581335		
179	15.3		12.3	18.5
176	18.5		15.0	22.6

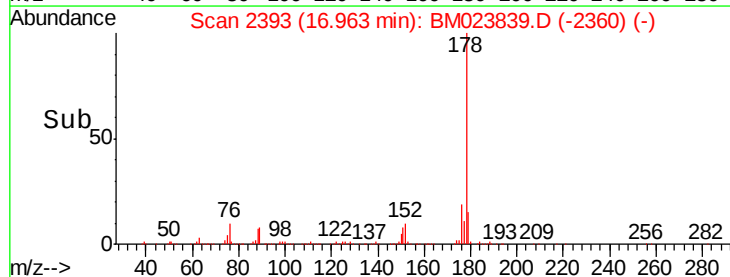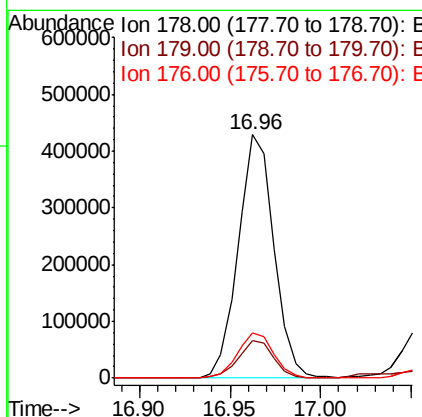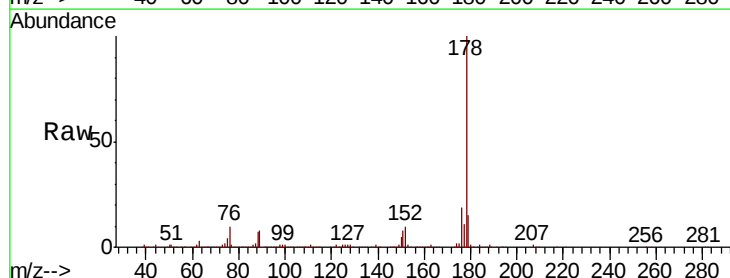

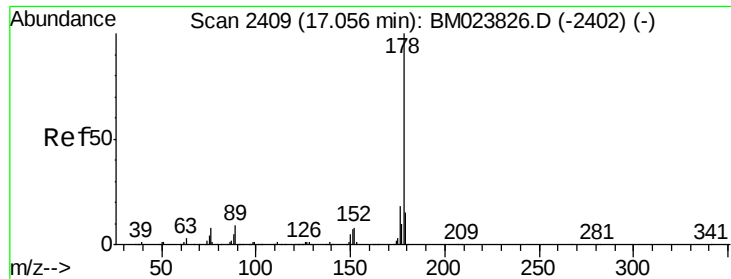





#72
 Anthracene
 Concen: 1.305 ng/ul
 RT: 17.06 min Scan# 2409
 Delta R.T. -0.01 min
 Lab File: BM023839.D
 Acq: 21 Nov 2019 21:07

Instrument :
 BNA_M
 ClientSampleId :
 C0AB2

Tot Ion	Ratio	Lower	Upper
178	100		
179	16.7	12.3	18.5
176	20.6	14.7	22.1




Manual Integrations
 APPROVED


mohammad
 11/22/2019 1:22:51 PM

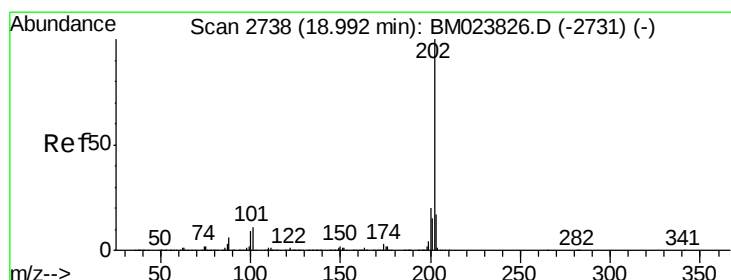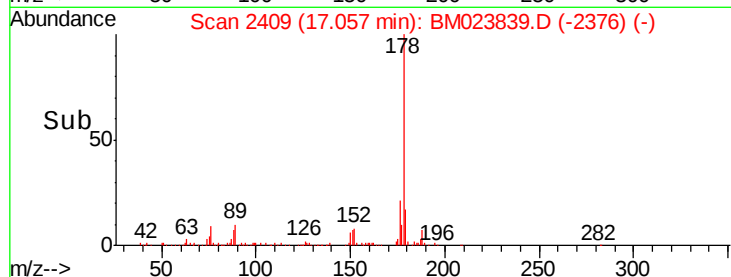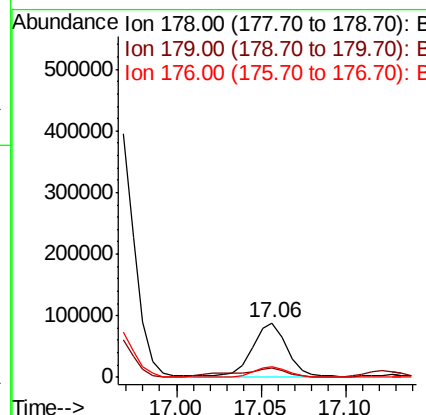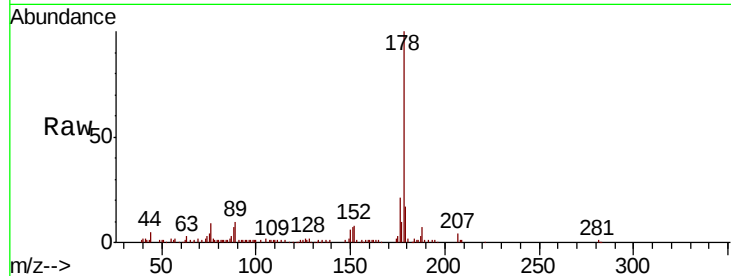

#77
 Fluoranthene
 Concen: 11.078 ng/ul
 RT: 18.99 min Scan# 2738
 Delta R.T. -0.01 min
 Lab File: BM023839.D
 Acq: 21 Nov 2019 21:07

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.4	7.7	11.5
100	8.7	6.0	9.0

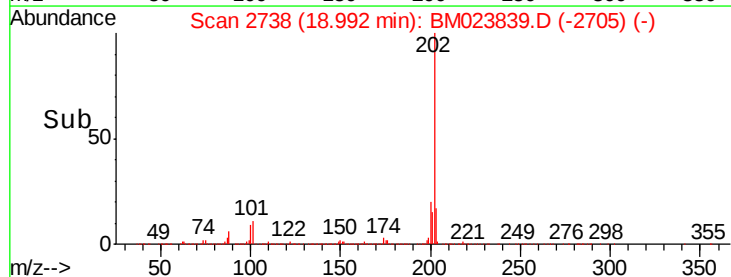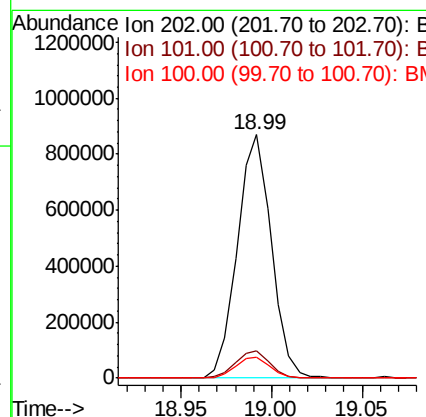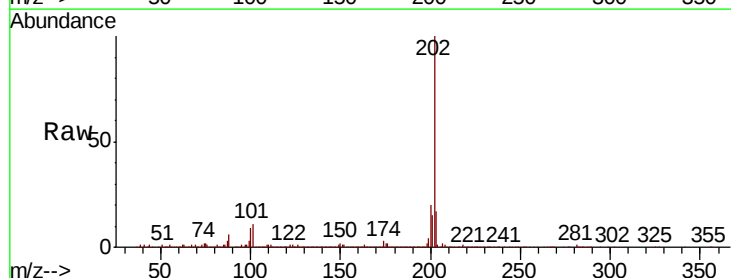

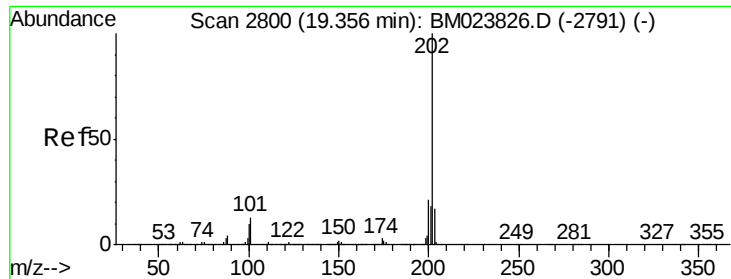





#80
Pvrene
Concen: 9.336 ng/ul
RT: 19.36 min Scan# 2800
Delta R.T. -0.01 min
Lab File: BM023839.D
Acq: 21 Nov 2019 21:07

Instrument :
BNA_M
ClientSampleId :
C0AB2

Tot Ion	Ratio	Lower	Upper
202	100		
101	12.8	9.8	14.6
100	11.2	8.1	12.1




Manual Integrations
APPROVED


mohammad
11/22/2019 1:22:51 PM

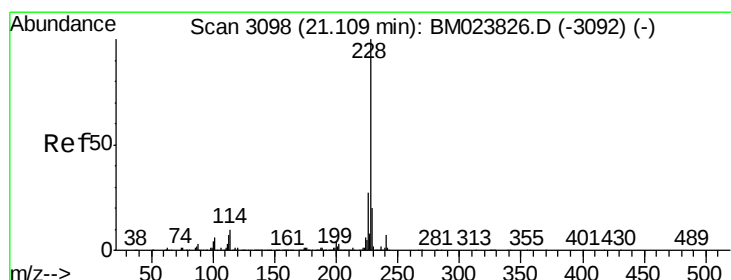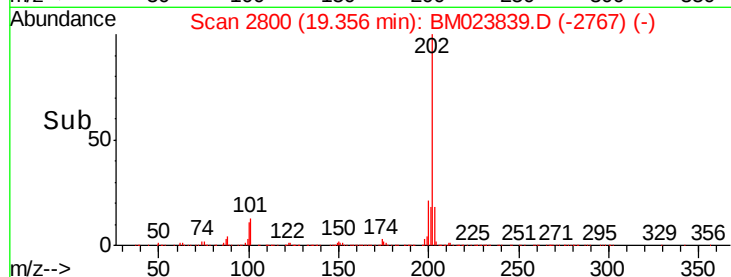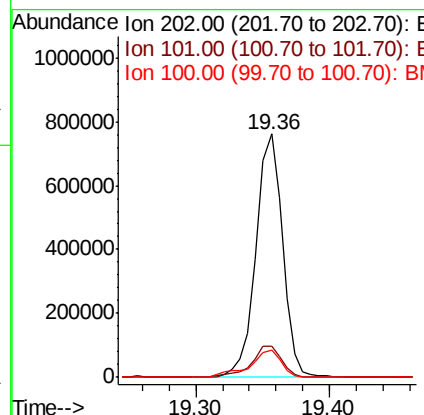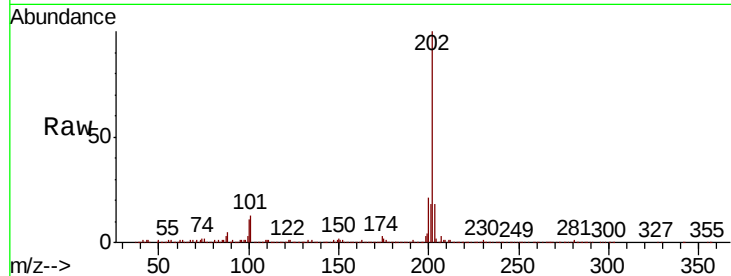

#83
Benzo(a)anthracene
Concen: 5.112 ng/ul
RT: 21.12 min Scan# 3099
Delta R.T. -0.01 min
Lab File: BM023839.D
Acq: 21 Nov 2019 21:07

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.6	15.6	23.4
226	27.5	21.4	32.2

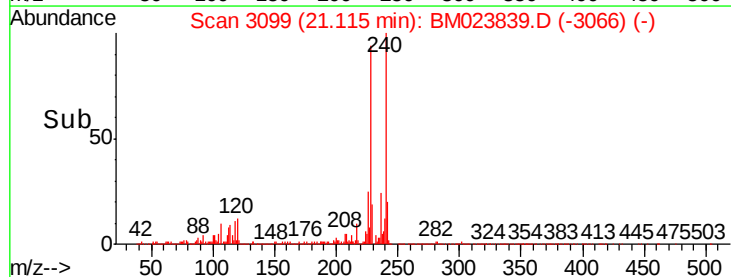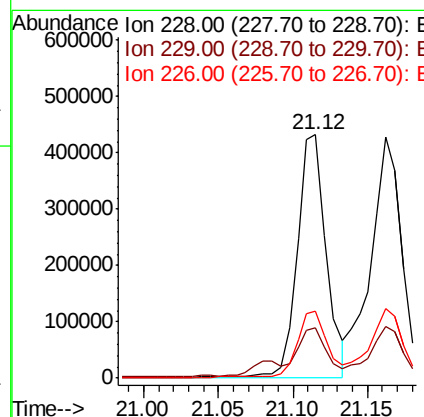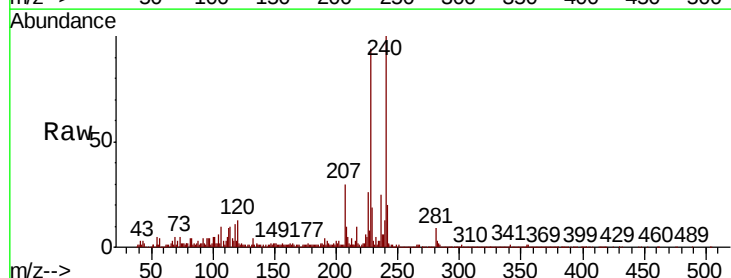

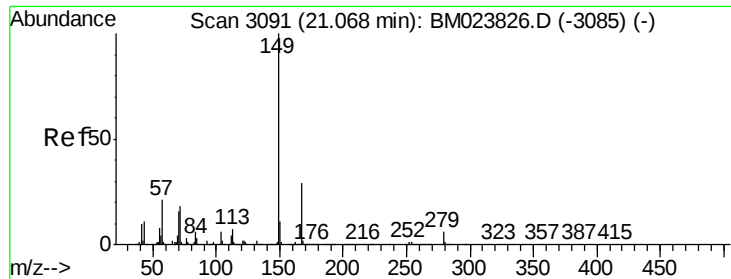

#84

Bis(2-ethylhexyl)phthalate

Concen: 1.260 ng/ul

RT: 21.07 min Scan# 3091

Delta R.T. -0.01 min

Lab File: BM023839.D

Acq: 21 Nov 2019 21:07

Instrument :

BNA_M





ClientSampleId :

C0AB2

Tot Ion:	149	Resp:	67411
Ion Ratio	Lower	Upper	
149	100		
167	29.1	23.4	35.2
279	7.1	5.0	7.4

Manual Integrations
APPROVED

mohammad
11/22/2019 1:22:51 PM

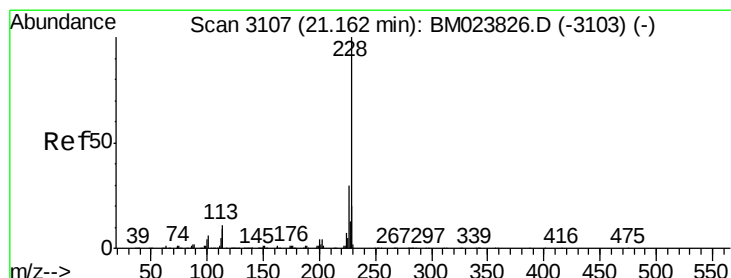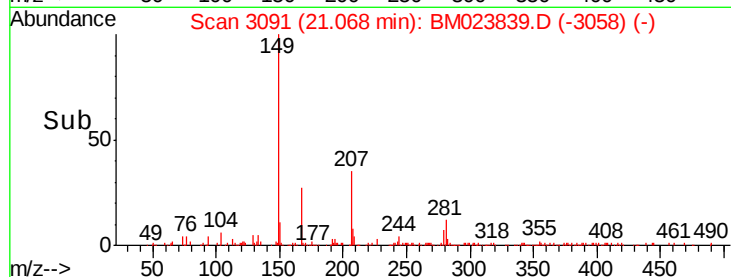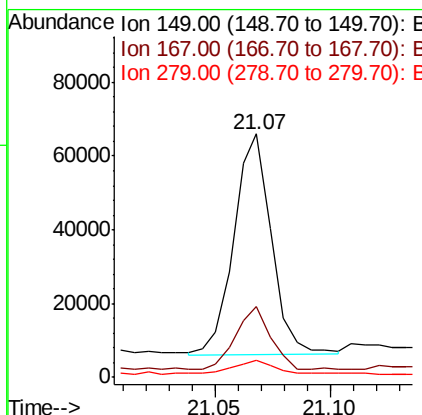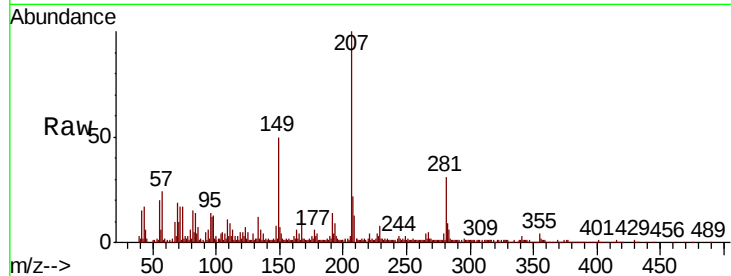

#85

Chrysene

Concen: 5.664 ng/ul




RT: 21.16 min Scan# 3107


Delta R.T. -0.01 min

Lab File: BM023839.D

Acq: 21 Nov 2019 21:07

Tgt Ion:	228	Resp:	608607
Ion Ratio	Lower	Upper	
228	100		
226	28.8	23.8	35.8
229	21.6	15.8	23.6

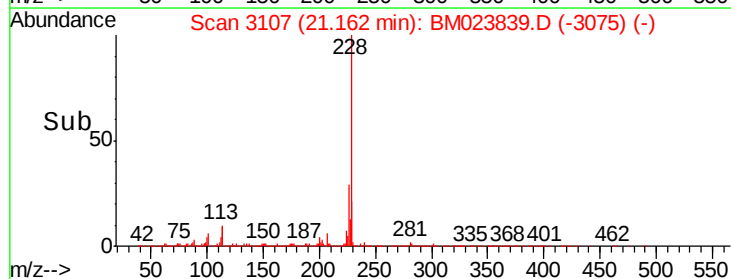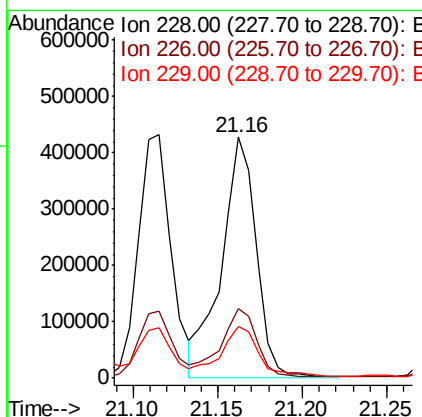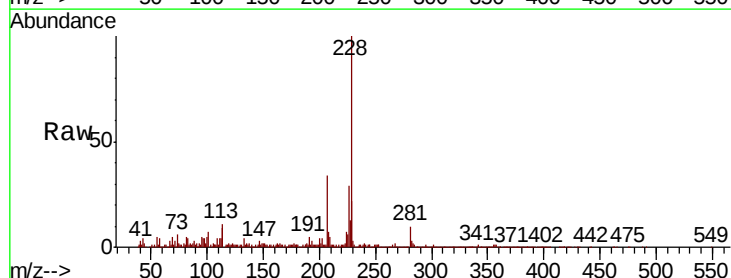

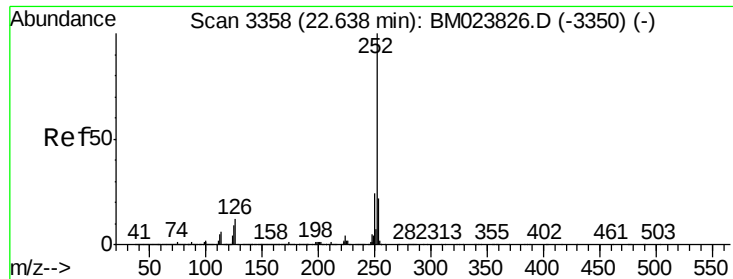





#88
Benzo(b)fluoranthene
Concen: 5.835 ng/ul
RT: 22.64 min Scan# 3359
Delta R.T. -0.01 min
Lab File: BM023839.D
Acq: 21 Nov 2019 21:07

Instrument :
BNA_M
ClientSampleID :
C0AB2

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.8	26.8
125	10.3	6.5	9.7




Manual Integrations
APPROVED


mohammad
11/22/2019 1:22:51 PM

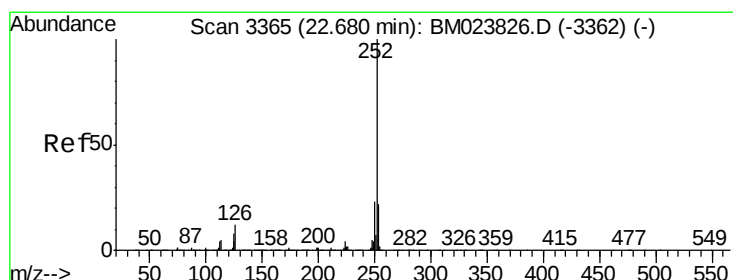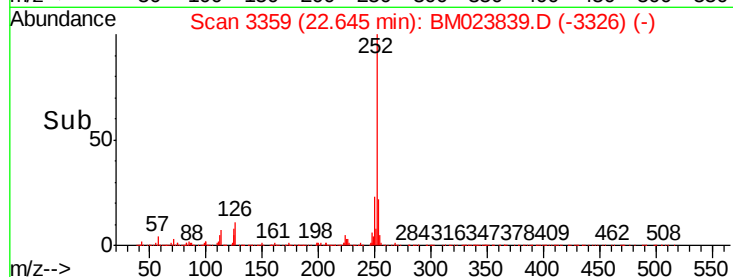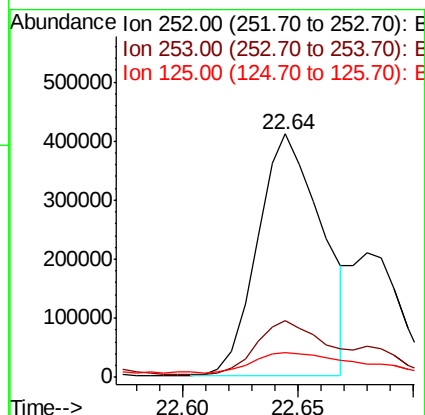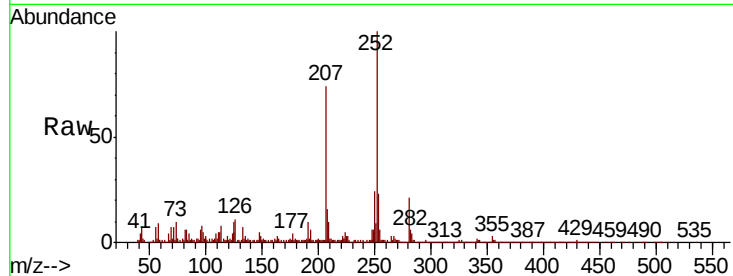

#89
Benzo(k)fluoranthene
Concen: 2.338 ng/ul m
RT: 22.68 min Scan# 3365
Delta R.T. -0.02 min
Lab File: BM023839.D
Acq: 21 Nov 2019 21:07

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.9	17.2	25.8
125	11.1	5.9	8.9

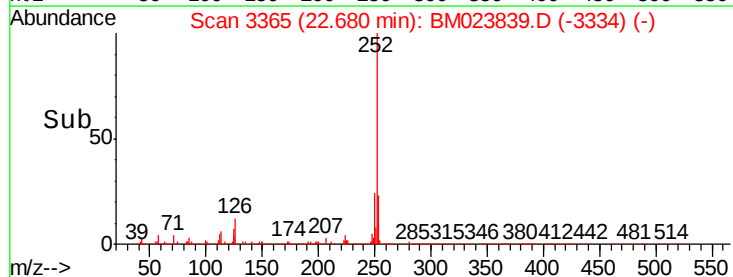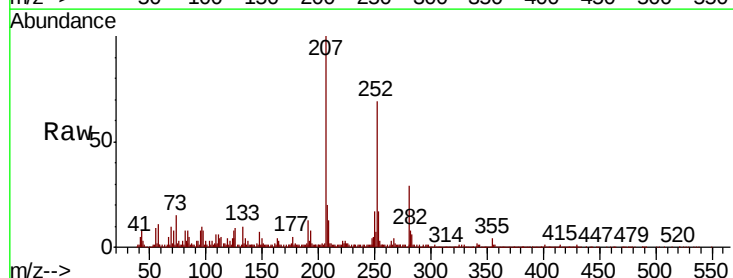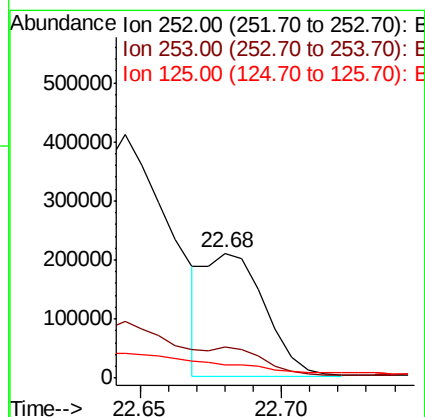

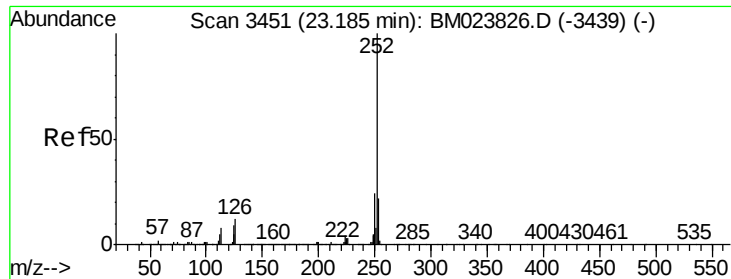

#91

Benzo(a)pyrene

Concen: 4.728 ng/ul

RT: 23.19 min Scan# 3452

Delta R.T. -0.01 min

Lab File: BM023839.D

Acq: 21 Nov 2019 21:07

Instrument :

BNA_M





ClientSampleId :

C0AB2

Tot Ion	Ratio	Resp	Lower	Upper
252	100	589419		
253	23.8	17.3	25.9	
125	11.3	6.9	10.3	

Manual Integrations
APPROVED

mohammad
11/22/2019 1:22:51 PM

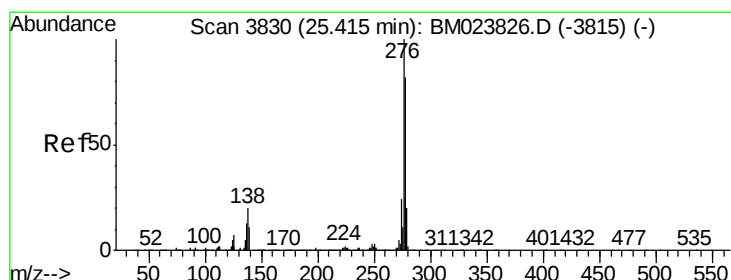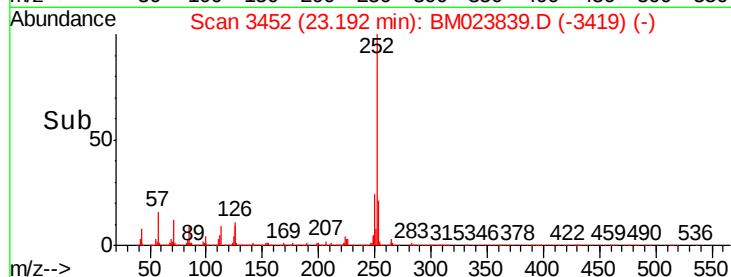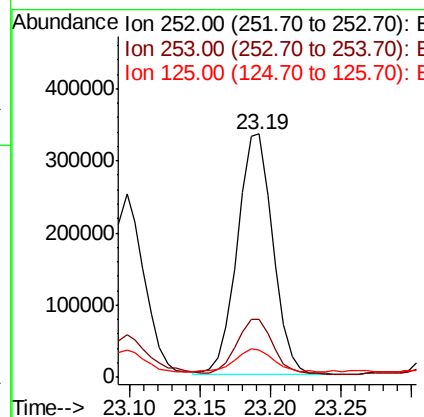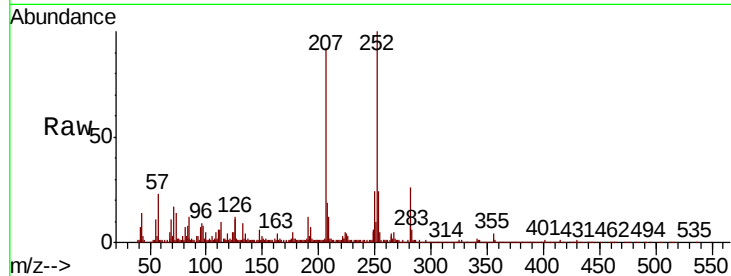

#92

Indeno(1,2,3-cd)pyrene

Concen: 3.341 ng/ul




RT: 25.41 min Scan# 3830


Delta R.T. -0.02 min

Lab File: BM023839.D

Acq: 21 Nov 2019 21:07

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	445425		
138	17.4	15.0	22.4	
277	25.4	20.0	30.0	

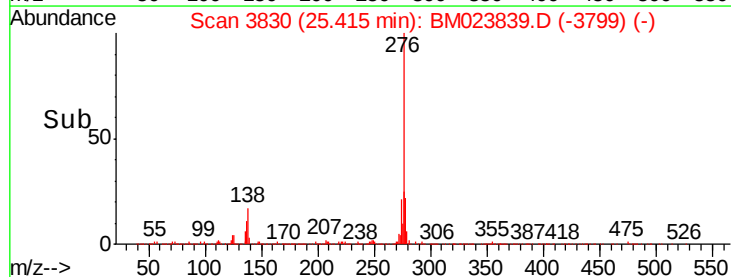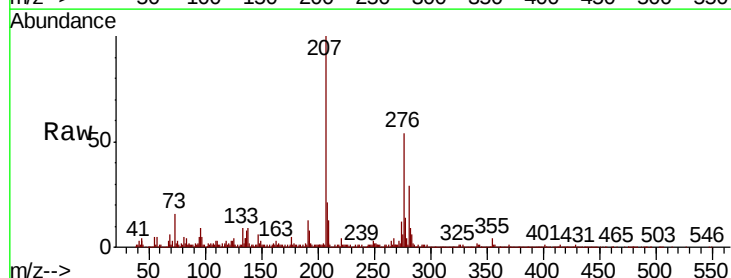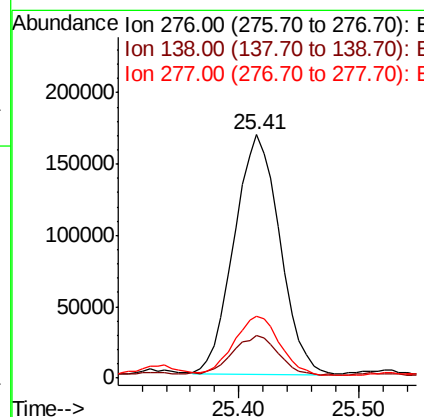

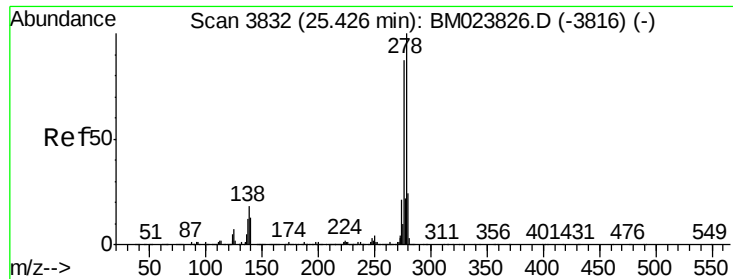





#93
Dibenzo(a,h)anthracene
Concen: 1.074 ng/ul
RT: 25.42 min Scan# 3831
Delta R.T. -0.02 min
Lab File: BM023839.D
Acq: 21 Nov 2019 21:07

Instrument :
BNA_M
ClientSampleId :
C0AB2

Tot Ion	Ratio	Lower	Upper
278	100		
139	20.1	10.0	15.0#
279	29.7	19.0	28.6#

Manual Integrations
APPROVED

mohammad
11/22/2019 1:22:51 PM

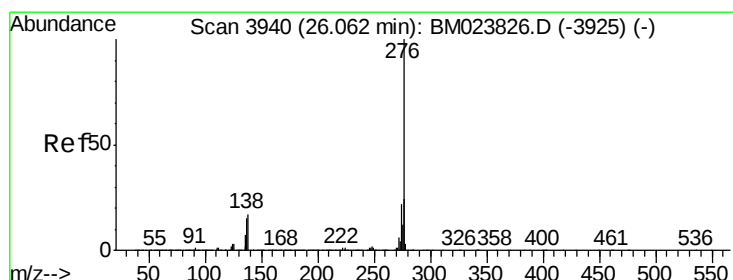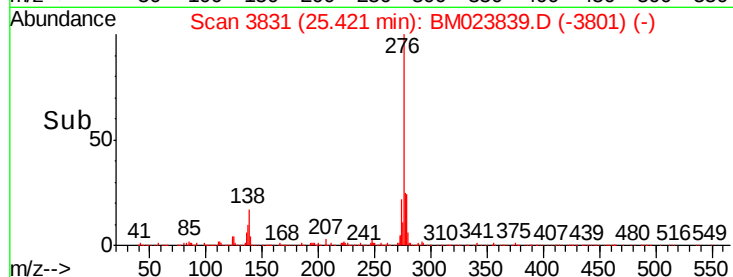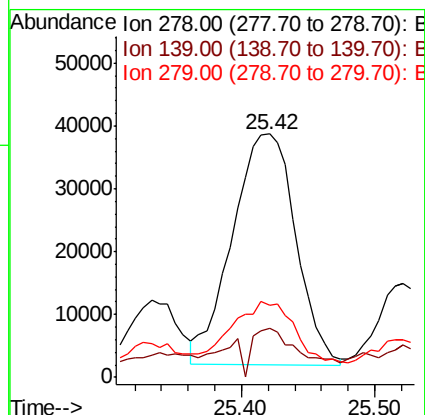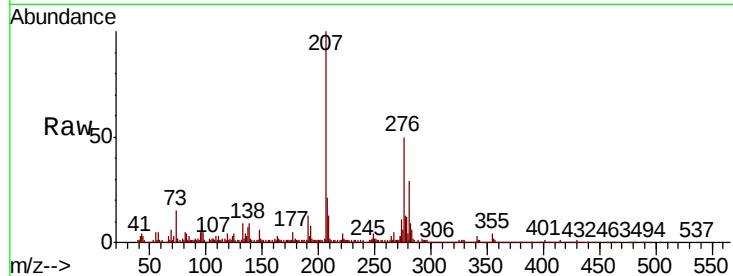

#94
Benzo(g,h,i)perylene
Concen: 4.188 ng/ul
RT: 26.07 min Scan# 3941
Delta R.T. -0.02 min
Lab File: BM023839.D
Acq: 21 Nov 2019 21:07

Tgt Ion	Ratio	Lower	Upper
276	100		
138	16.9	13.2	19.8
277	24.2	18.6	28.0

