

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112119\
 Data File : BM023851.D
 Acq On : 22 Nov 2019 04:56
 Operator : JU
 Sample : K5809-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFPT1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.975	11	15	25	rVB	867760	941928	21.10%	5.448%
2	3.275	62	66	68	rBV	80660	100381	2.25%	0.581%
3	3.299	68	70	77	rVB2	118968	131524	2.95%	0.761%
4	3.528	106	109	114	rVB2	26222	36318	0.81%	0.210%
5	3.622	122	125	129	rVB	27759	29520	0.66%	0.171%
6	3.669	129	133	139	rVB	50879	78835	1.77%	0.456%
7	3.763	145	149	157	rVB2	53636	81417	1.82%	0.471%
8	3.869	164	167	171	rVB	40790	50352	1.13%	0.291%
9	4.293	235	239	245	rVB4	31608	58002	1.30%	0.335%
10	4.398	252	257	260	rVB2	23508	30155	0.68%	0.174%
11	4.498	271	274	278	rVB2	26601	34488	0.77%	0.199%
12	4.593	285	290	294	rBV	78268	102033	2.29%	0.590%
13	4.904	339	343	348	rBV4	15659	25454	0.57%	0.147%
14	4.998	355	359	362	rBV4	18629	26537	0.59%	0.153%
15	5.328	411	415	421	rBV4	14127	29581	0.66%	0.171%
16	5.457	431	437	440	rBV6	14812	24037	0.54%	0.139%
17	5.534	446	450	461	rVB10	18020	44261	0.99%	0.256%
18	5.804	490	496	502	rVB5	18936	31007	0.69%	0.179%
19	6.528	616	619	624	rVB2	18300	29803	0.67%	0.172%
20	6.751	652	657	660	rBV3	16638	26944	0.60%	0.156%
21	7.169	723	728	733	rVB2	28796	47314	1.06%	0.274%
22	7.516	780	787	799	rBV	1609748	2525827	56.58%	14.609%
23	7.651	803	810	818	rVB4	19847	46805	1.05%	0.271%
24	10.292	1250	1259	1273	rBV	2056367	3478641	77.93%	20.119%
25	10.545	1298	1302	1310	rVB9	10424	23614	0.53%	0.137%
26	10.980	1370	1376	1383	rBV8	15754	30916	0.69%	0.179%
27	12.957	1705	1712	1718	rBV9	20429	47974	1.07%	0.277%
28	13.598	1816	1821	1825	rBV4	32960	55672	1.25%	0.322%
29	13.921	1871	1876	1878	rBV6	20081	37763	0.85%	0.218%
30	14.010	1887	1891	1896	rVB6	38719	58699	1.32%	0.339%
31	14.180	1910	1920	1930	rBV	2889613	4428134	99.20%	25.611%
32	14.268	1930	1935	1941	rBV7	23121	41313	0.93%	0.239%
33	14.510	1972	1976	1982	rBV7	19614	35487	0.79%	0.205%
34	14.974	2052	2055	2059	rBV3	41970	55549	1.24%	0.321%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112119\
Data File : BM023851.D
Acq On : 22 Nov 2019 04:56
Operator : JU
Sample : K5809-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFPT1

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Title : SVOA CALIBRATION

35	16.927	2382	2387	2397	rBV	3014220	4463779	100.00%	25.817%
----	--------	------	------	------	-----	---------	---------	---------	---------


Sum of corrected areas: 17290064

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112119\
Data File : BM023851.D
Acq On : 22 Nov 2019 04:56
Operator : JU
Sample : K5809-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFPT1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

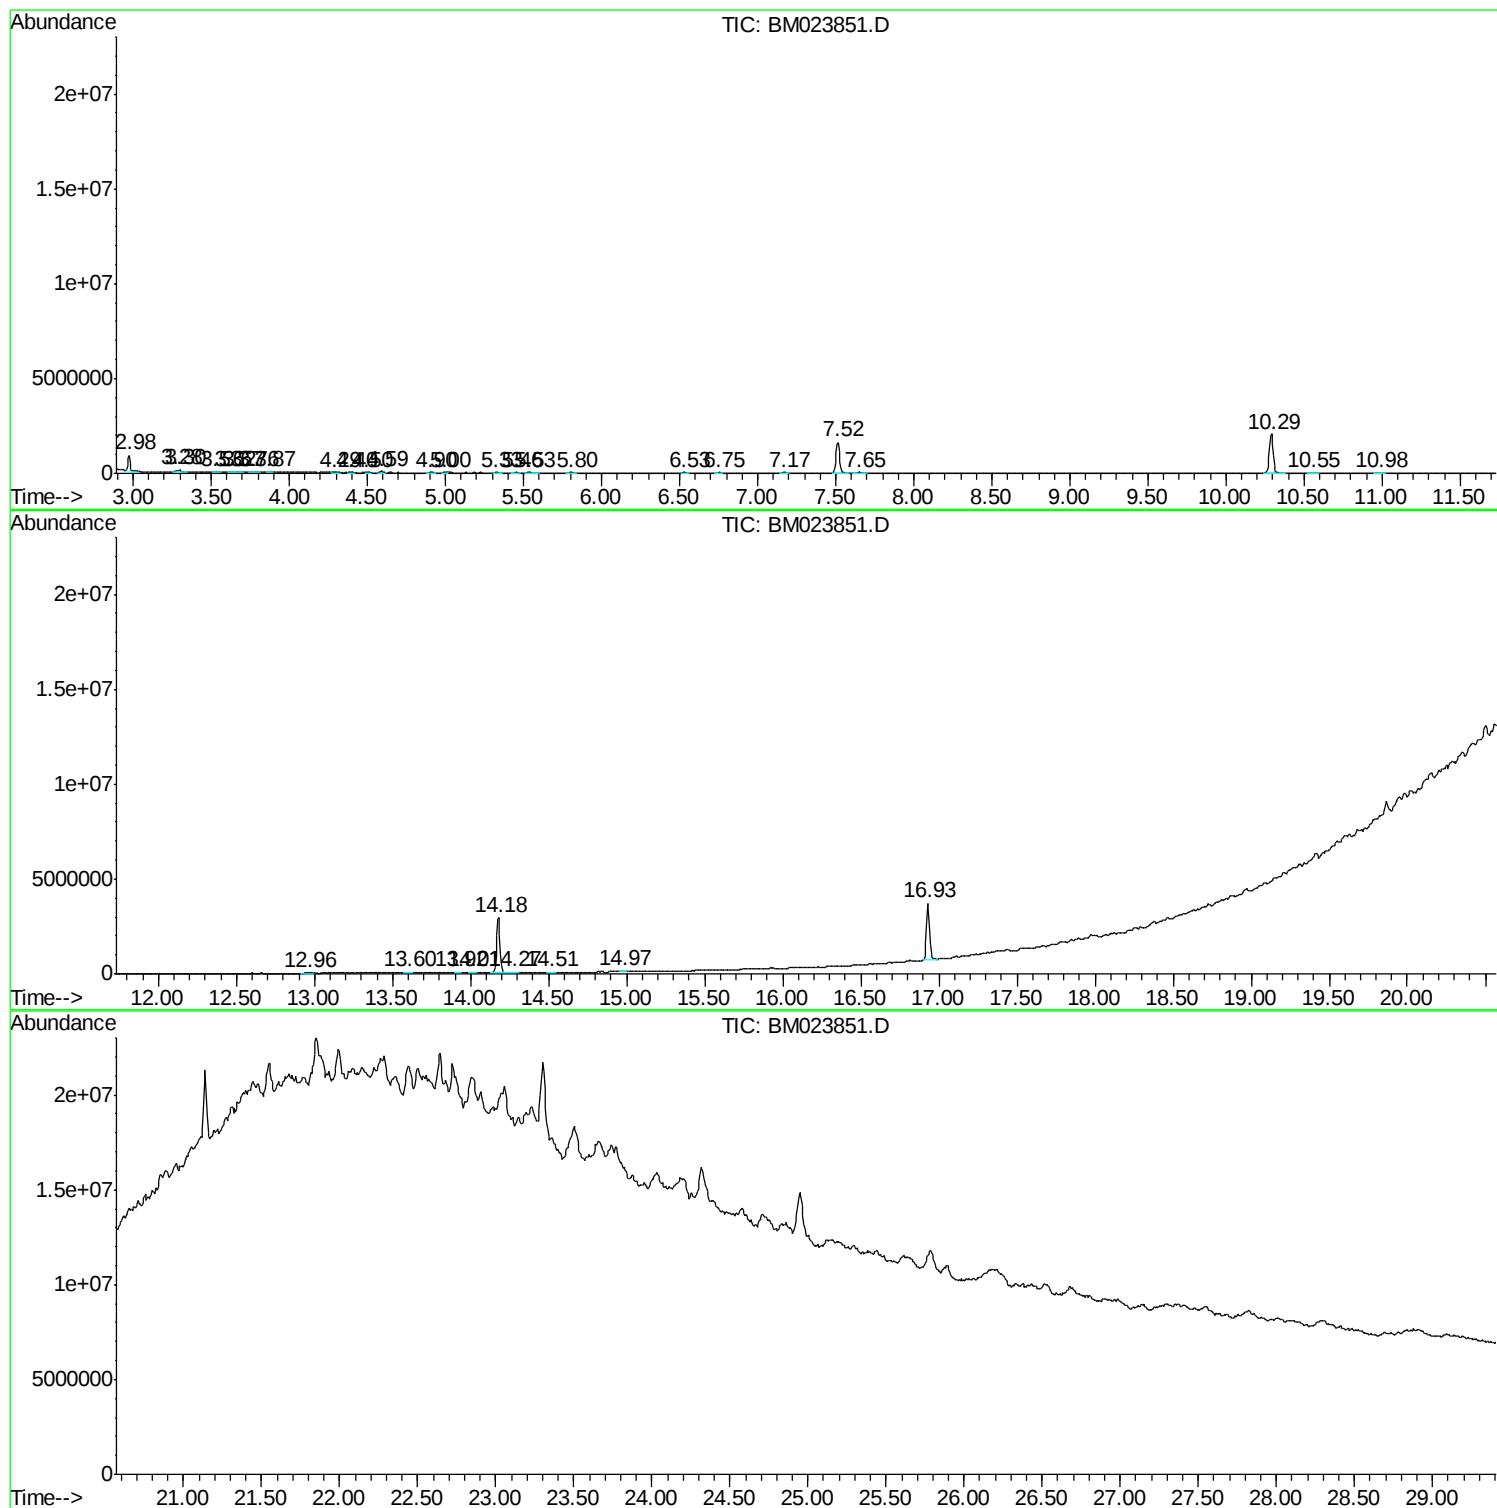

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112119\
Data File : BM023851.D
Acq On : 22 Nov 2019 04:56
Operator : JU
Sample : K5809-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFPT1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.98	7.46 ng/ul	941928	1,4-Dichlorobenzene-d4	7.52

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	91
2		Heptane	100	C7H16	000142-82-5	91
3		Heptane	100	C7H16	000142-82-5	91
4		Heptane	100	C7H16	000142-82-5	91
5		2-Bromononane	206	C9H19Br	002216-35-5	59

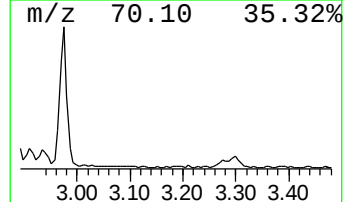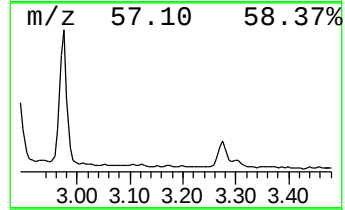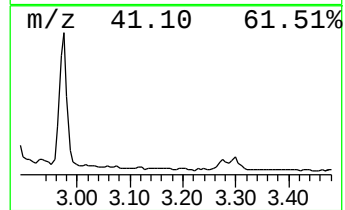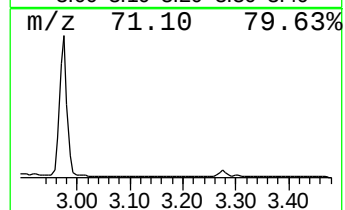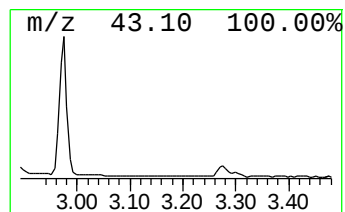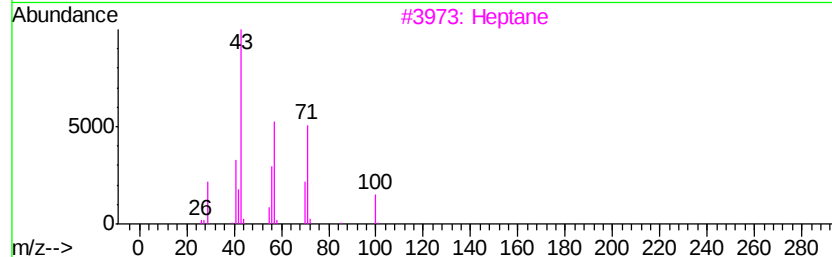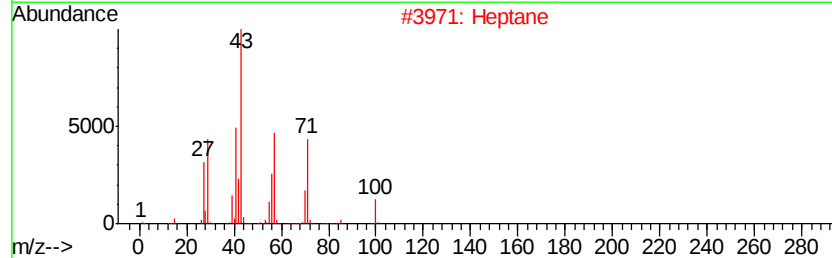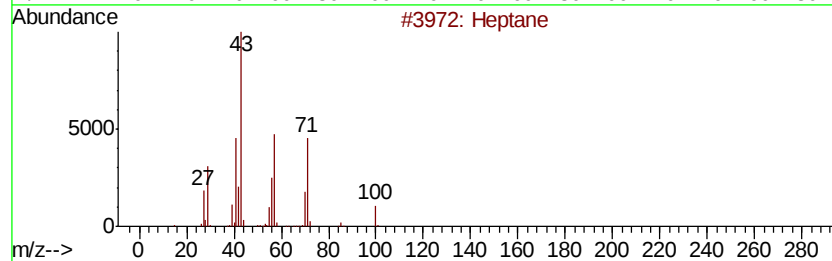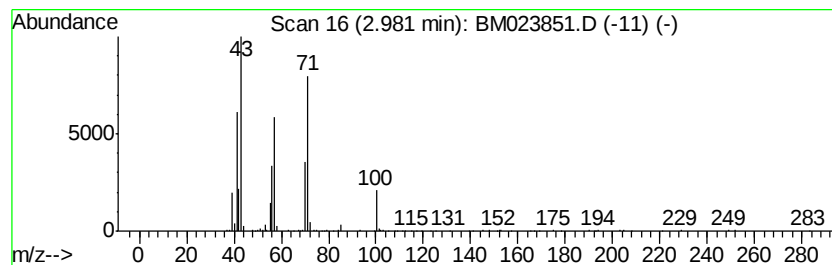

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112119\
Data File : BM023851.D
Acq On : 22 Nov 2019 04:56
Operator : JU
Sample : K5809-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFPT1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	2.98	7.5	ng/ul	941928	1	7.52	2525830	20.0