
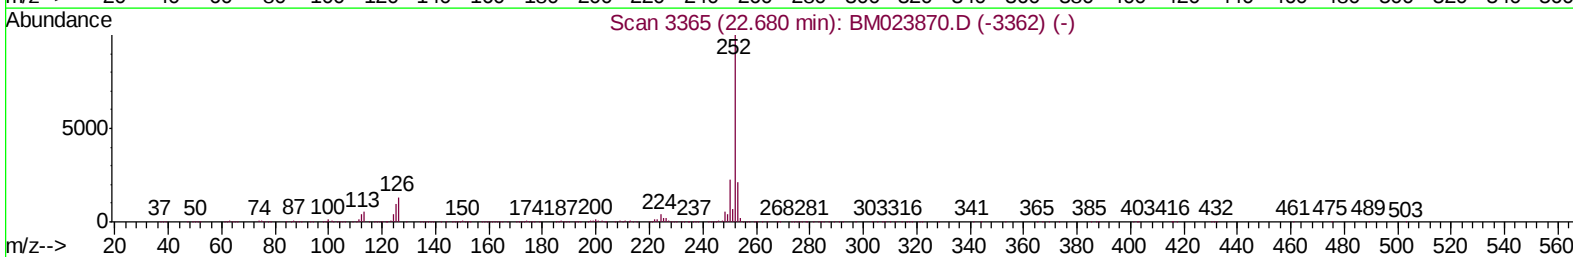
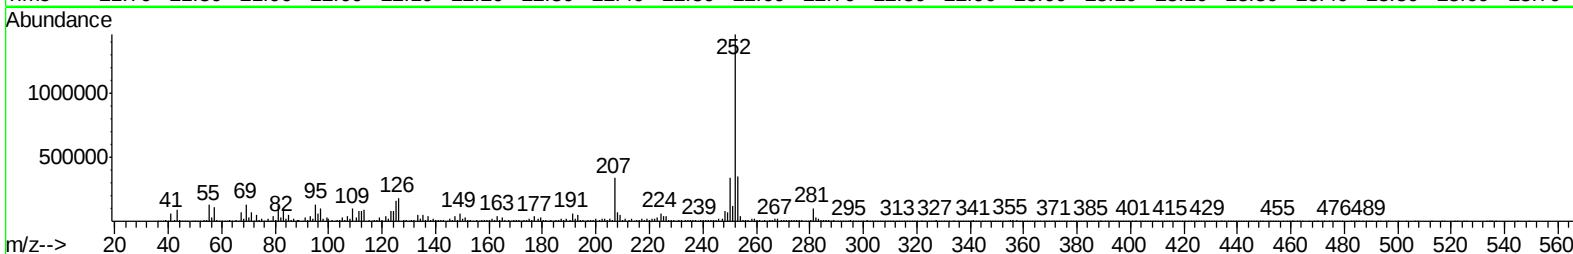


Data File : BM023879.D
Acq On : 23 Nov 2019 04:33
Operator : JU
Sample : K5854-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 25 01:12:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 25 01:09:42 2019
Response via : Initial Calibration

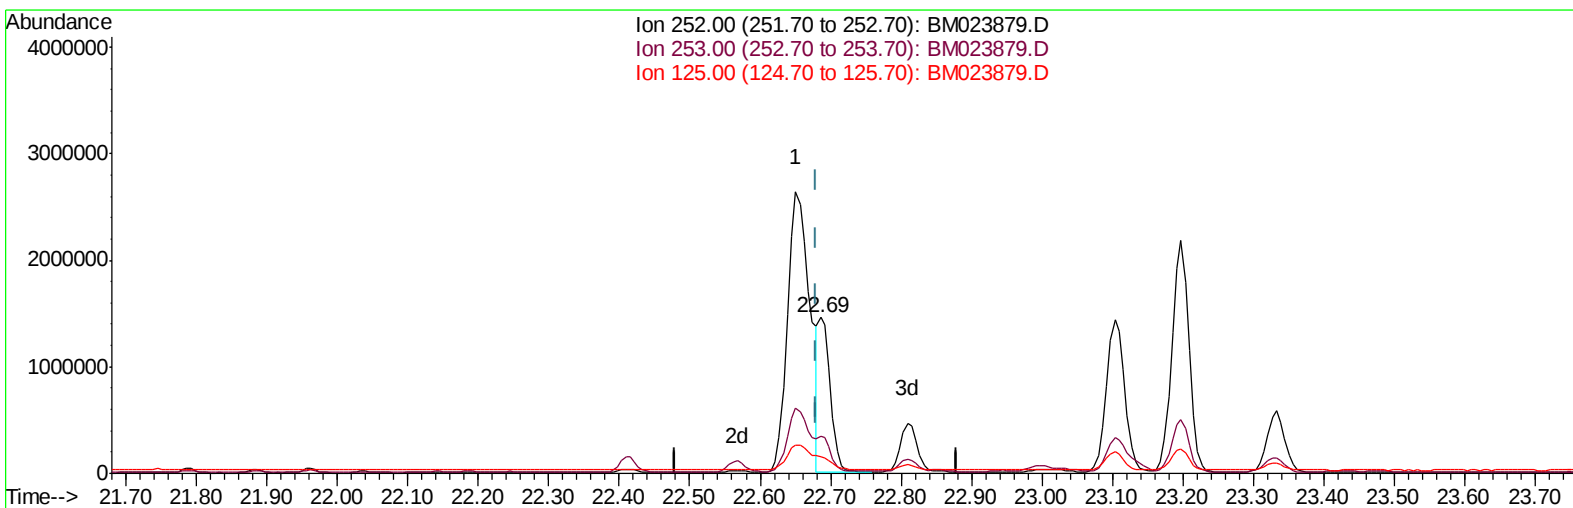

TIC: BM023879.D

(89) Benzo(k)fluoranthene

22.686min (+0.006) 11.16ng/ul m

response 1624847

Ion	Exp%	Act%
252.00	100	100
253.00	21.50	24.13
125.00	7.40	10.98#
0.00	0.00	0.00