
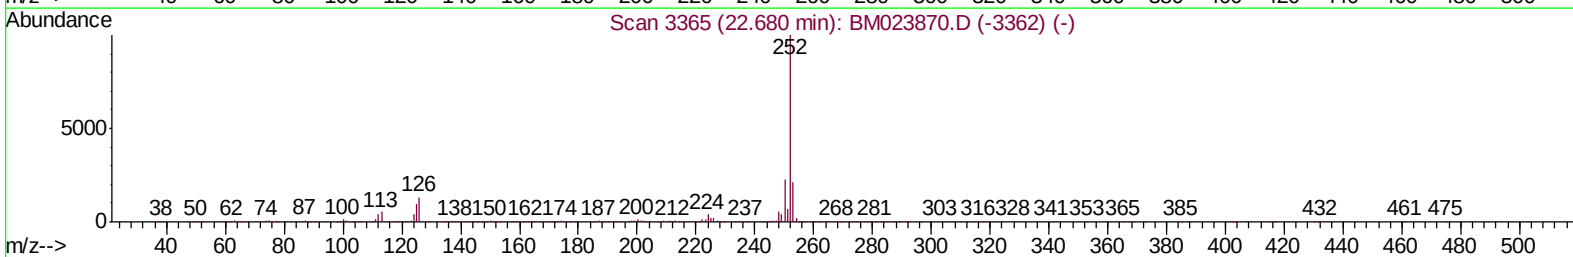
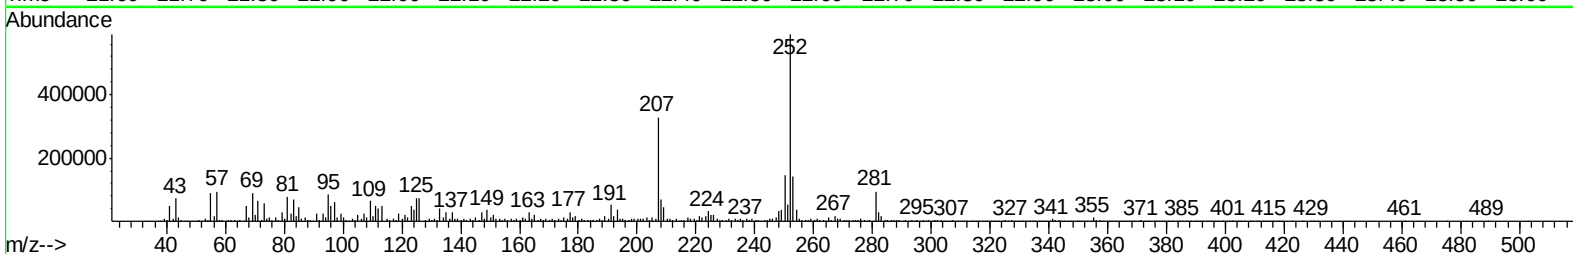


Data File : BM023872.D
Acq On : 23 Nov 2019 00:22
Operator : JU
Sample : K5854-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Nov 25 01:01:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 23 05:21:37 2019
Response via : Initial Calibration

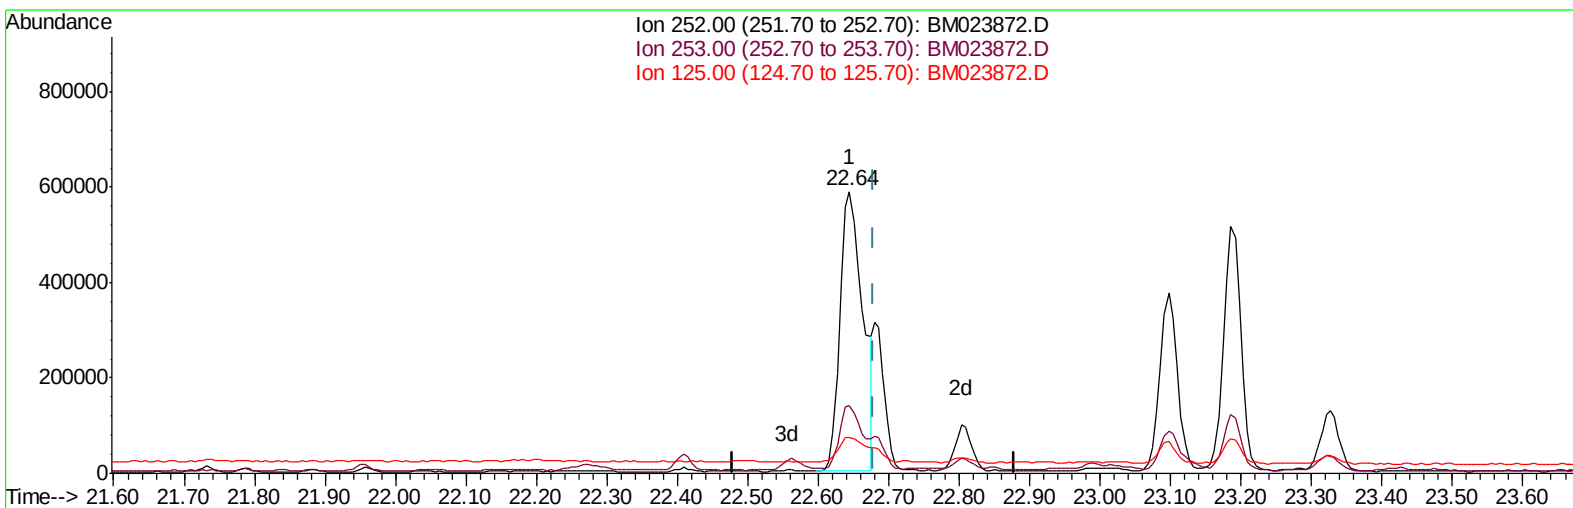

TIC: BM023872.D

(89) Benzo(k)fluoranthene
22.644min (-0.036) 9.21ng/ul
response 1306345

Ion	Exp%	Act%
252.00	100	100
253.00	21.50	23.97
125.00	7.40	12.72#
0.00	0.00	0.00