
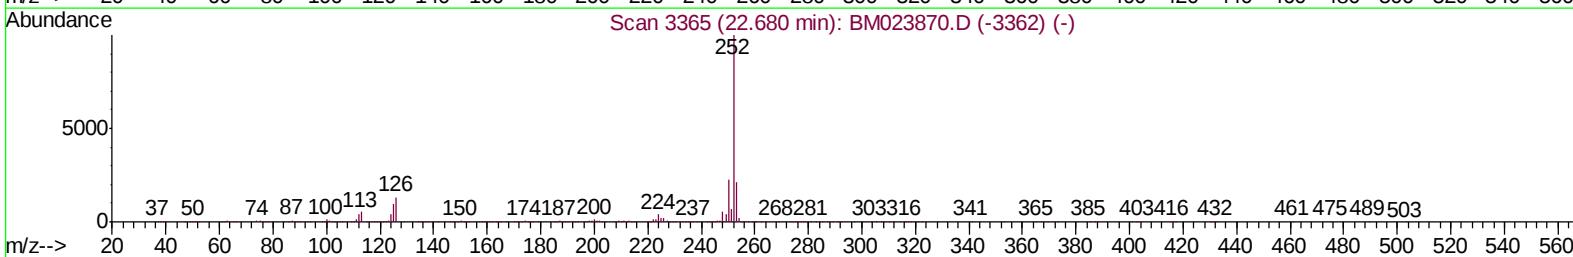
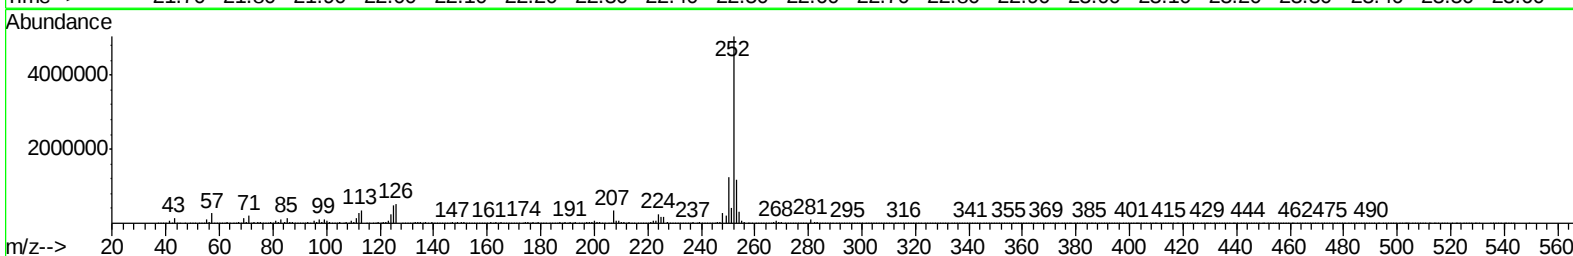


Data File : BM023874.D
Acq On : 23 Nov 2019 01:34
Operator : JU
Sample : K5854-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 23 05:25:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 23 05:21:37 2019
Response via : Initial Calibration

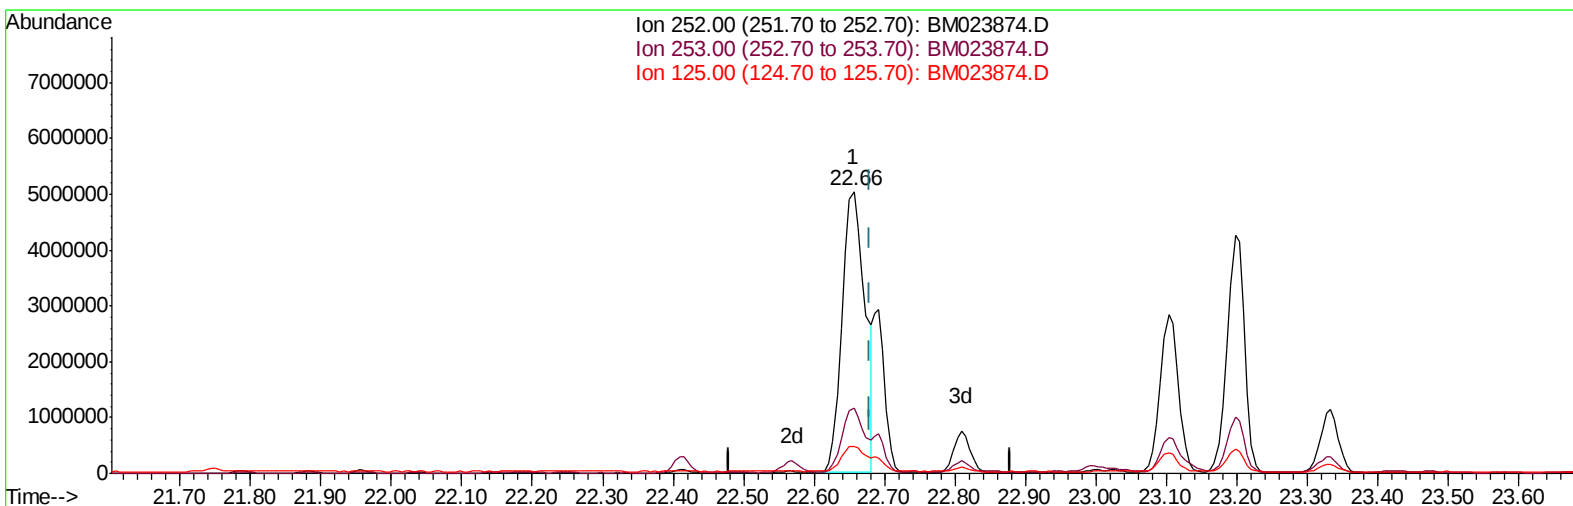

TIC: BM023874.D

(89) Benzo(k)fluoranthene

22.656min (-0.024) 76.39ng/ul

response 11283290

Ion	Exp%	Act%
252.00	100	100
253.00	21.50	23.09
125.00	7.40	9.59#
0.00	0.00	0.00