
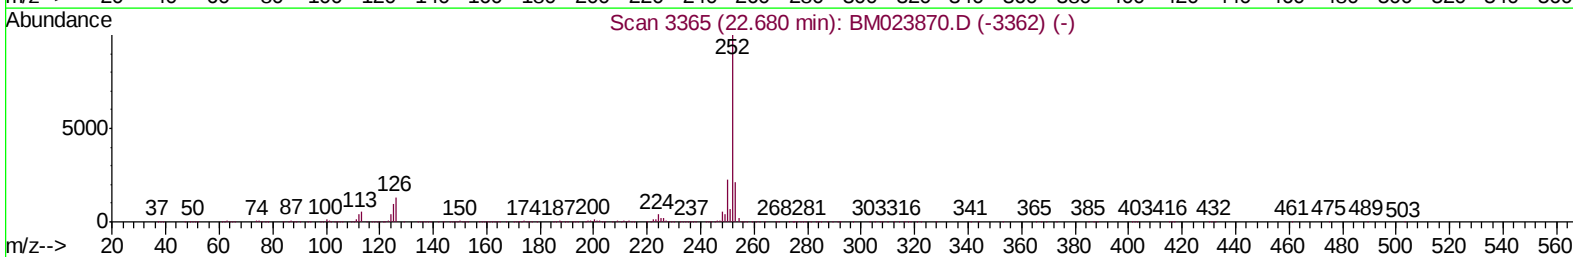
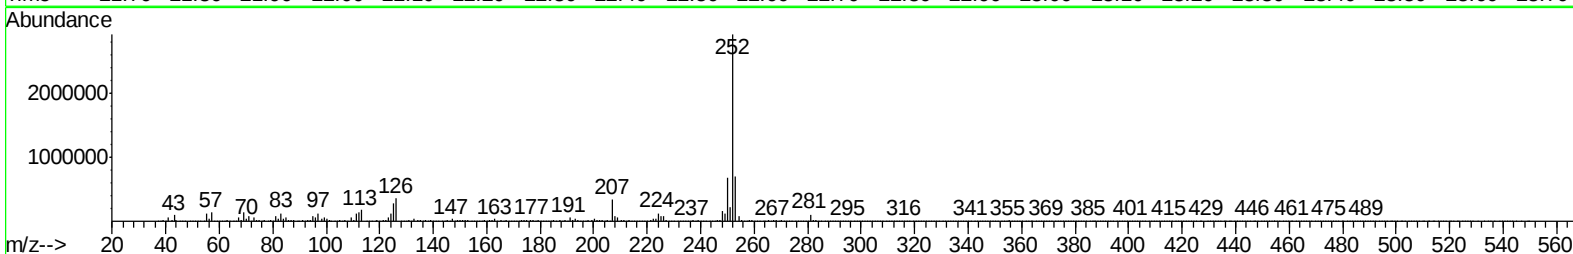


Data File : BM023874.D
Acq On : 23 Nov 2019 01:34
Operator : JU
Sample : K5854-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 23 05:25:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 23 05:21:37 2019
Response via : Initial Calibration

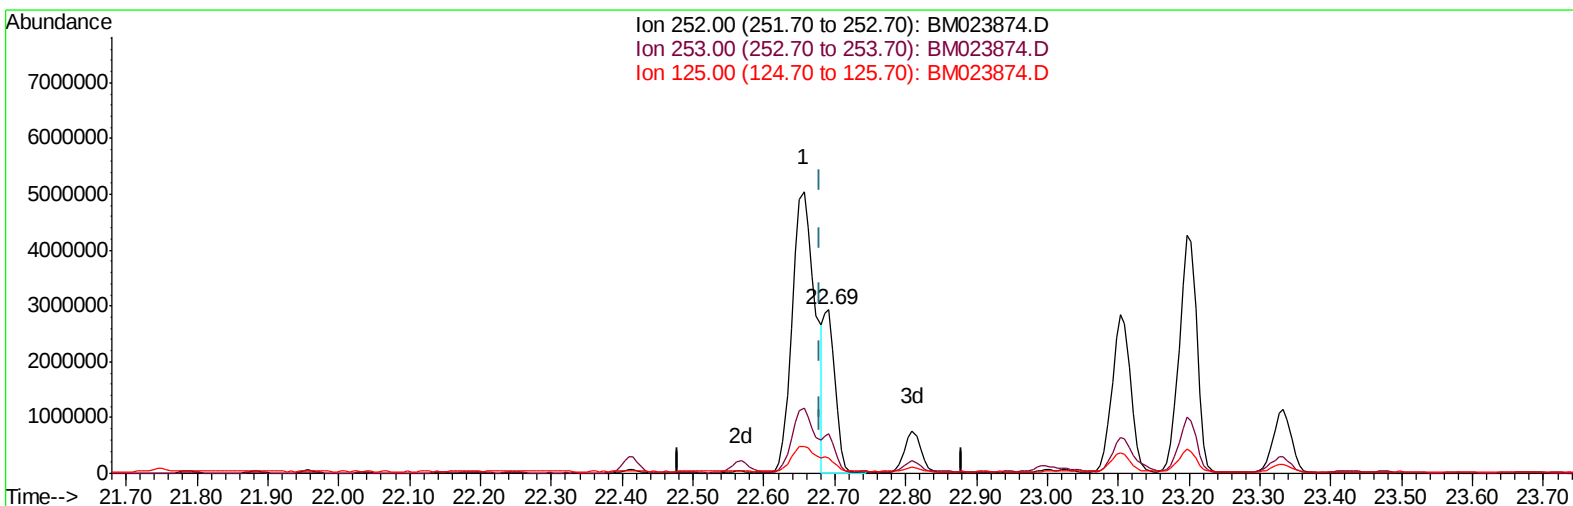

TIC: BM023874.D

(89) Benzo(k)fluoranthene

22.692min (+0.012) 23.23ng/ul m

response 3431092

Ion	Exp%	Act%
252.00	100	100
253.00	21.50	24.05
125.00	7.40	9.71#
0.00	0.00	0.00