
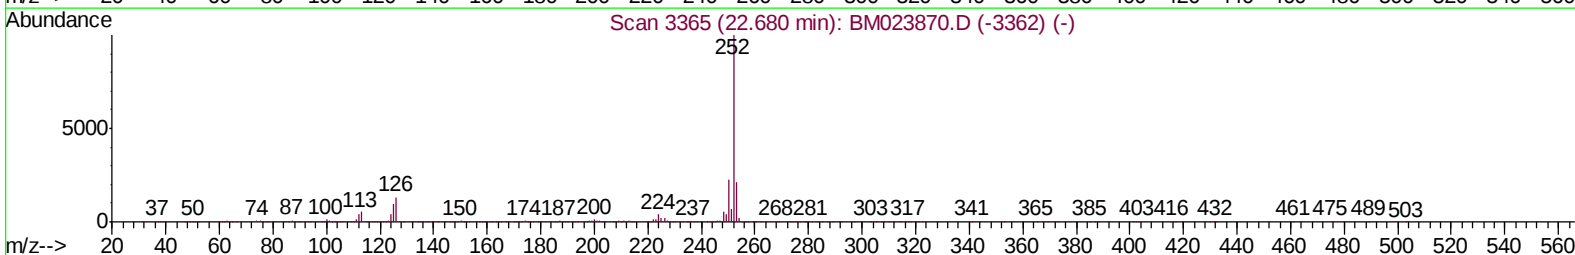
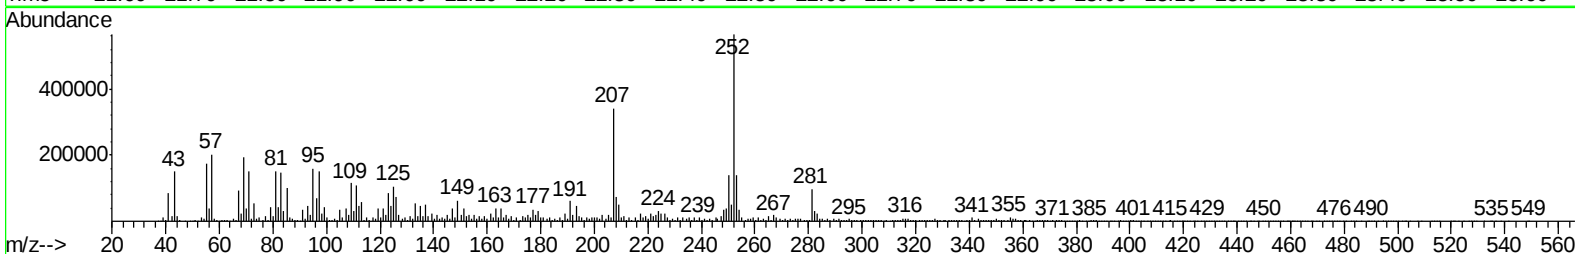


Data File : BM023877.D
Acq On : 23 Nov 2019 03:21
Operator : JU
Sample : K5854-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Nov 23 05:26:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 23 05:21:37 2019
Response via : Initial Calibration

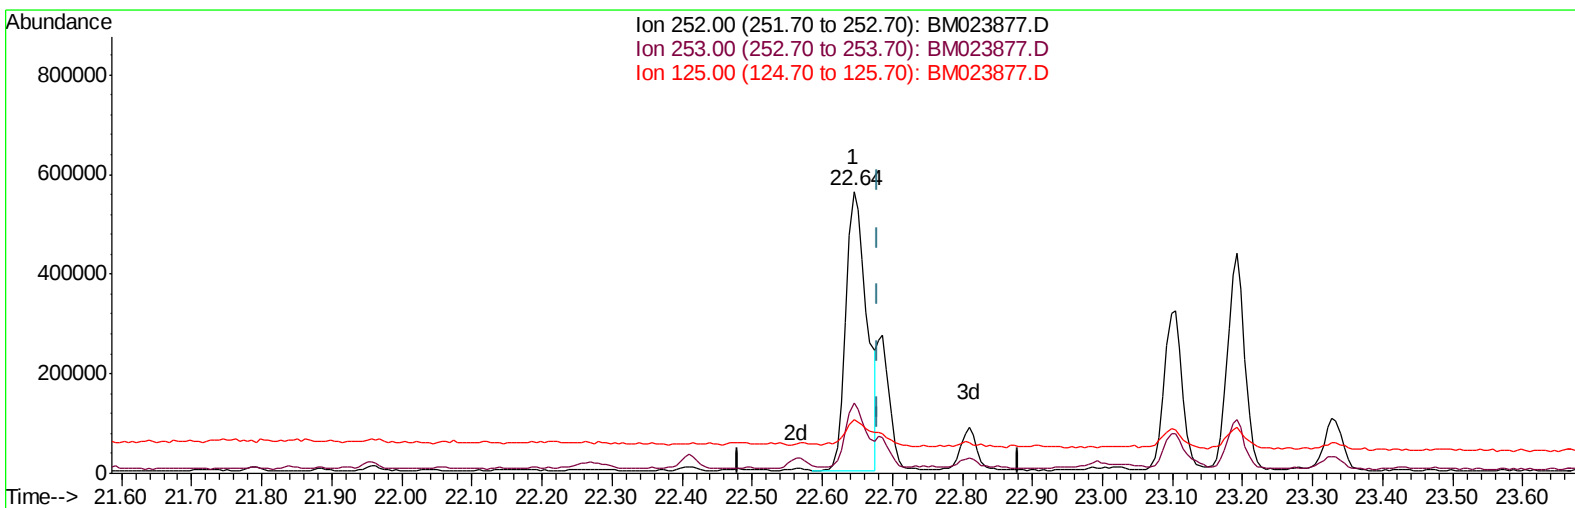

TIC: BM023877.D

(89) Benzo(k)fluoranthene
22.645min (-0.035) 7.89ng/ul
response 1157706

Ion	Exp%	Act%
252.00	100	100
253.00	21.50	24.80
125.00	7.40	18.88#
0.00	0.00	0.00