
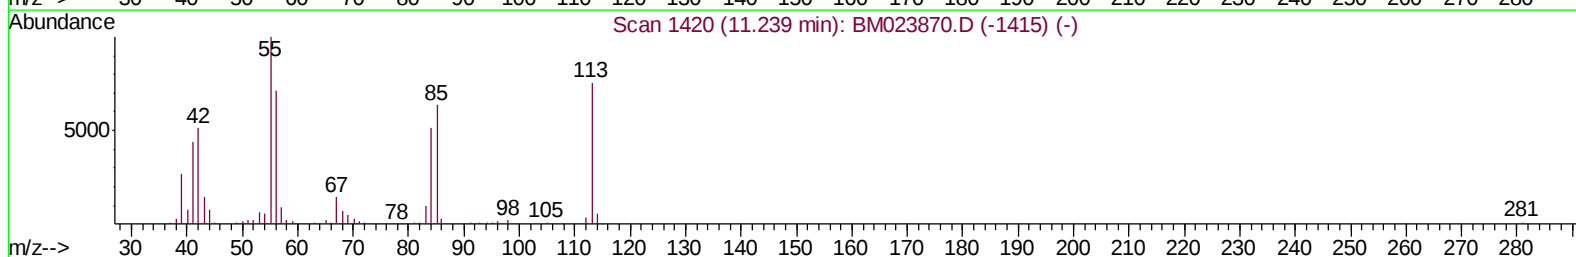
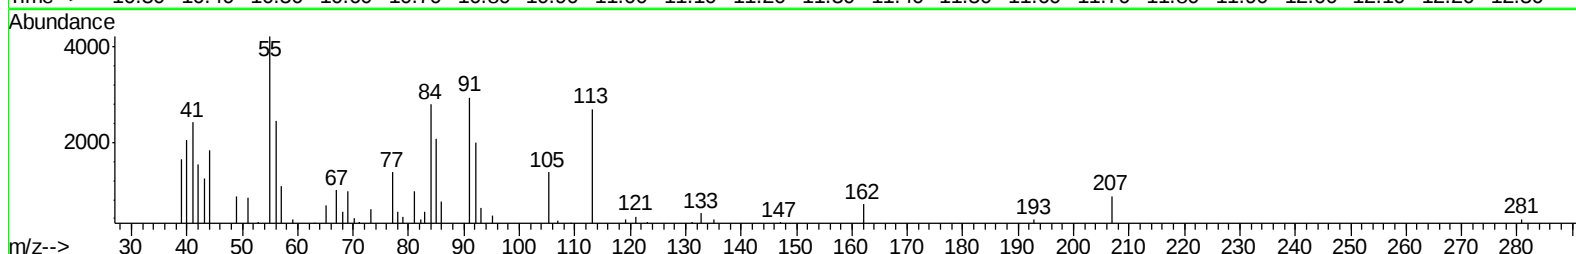


Data File : BM023878.D
Acq On : 23 Nov 2019 03:57
Operator : JU
Sample : K5854-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Nov 23 06:13:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 23 05:21:37 2019
Response via : Initial Calibration

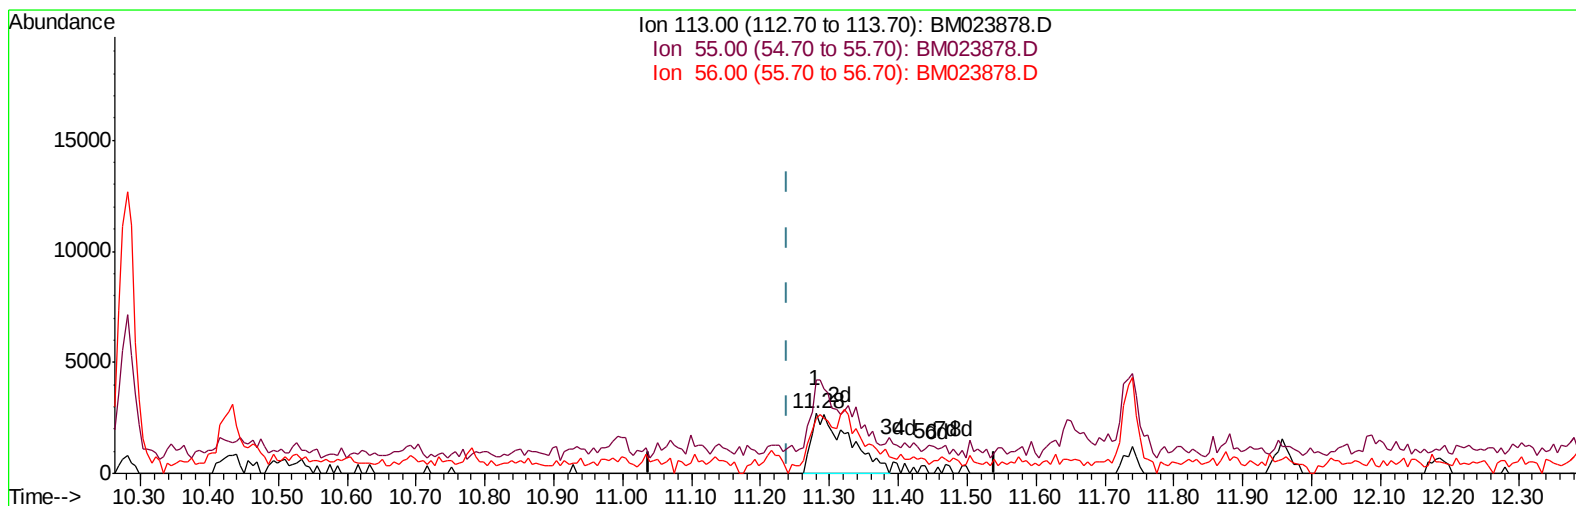

TIC: BM023878.D

(32) Caprolactam

11.280min (+0.041) 1.19ng/ul m

response 10245

Ion	Exp%	Act%
113.00	100	100
55.00	132.20	156.42
56.00	103.80	90.82
0.00	0.00	0.00