
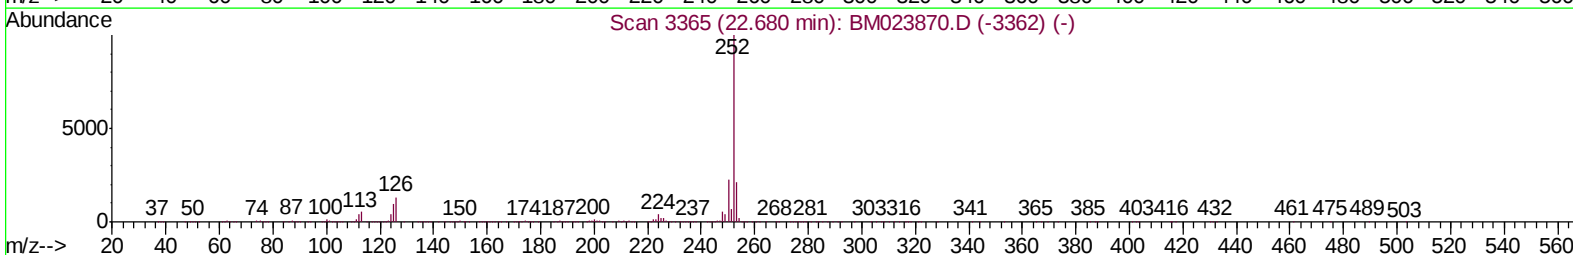
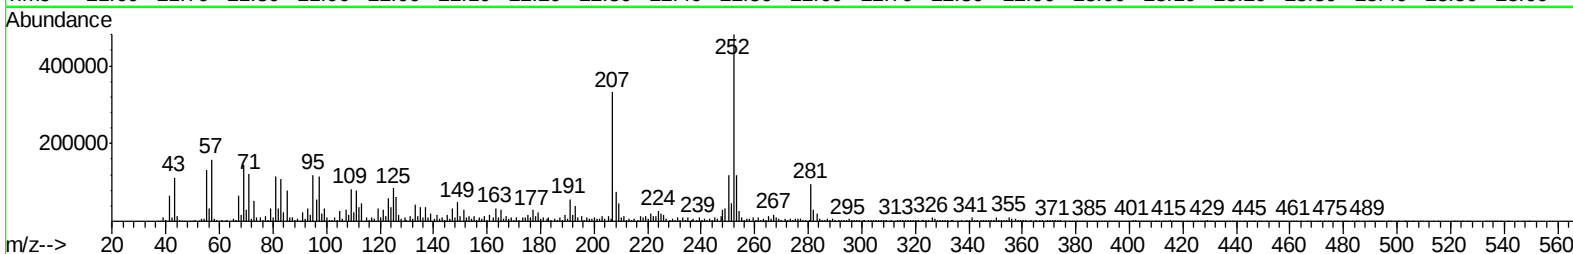


Data File : BM023878.D
Acq On : 23 Nov 2019 03:57
Operator : JU
Sample : K5854-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Nov 23 06:13:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 23 05:21:37 2019
Response via : Initial Calibration

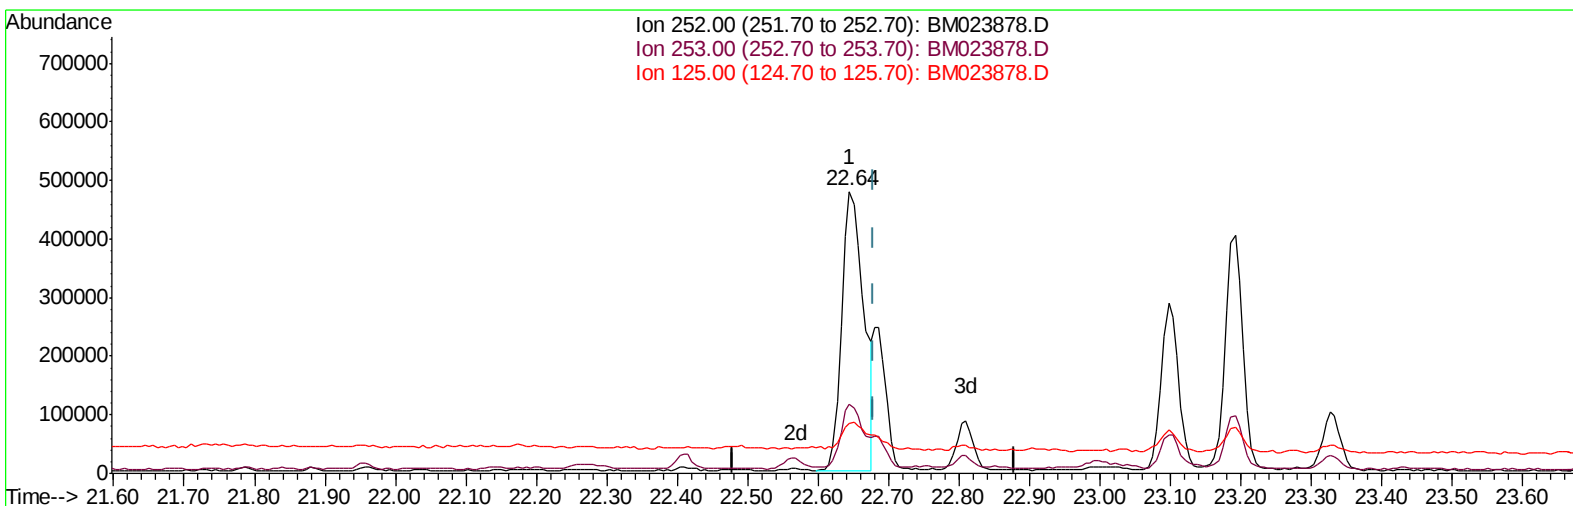

TIC: BM023878.D

(89) Benzo(k)fluoranthene
22.644min (-0.035) 6.65ng/ul
response 1018784

Ion	Exp%	Act%
252.00	100	100
253.00	21.50	24.77
125.00	7.40	17.57#
0.00	0.00	0.00