
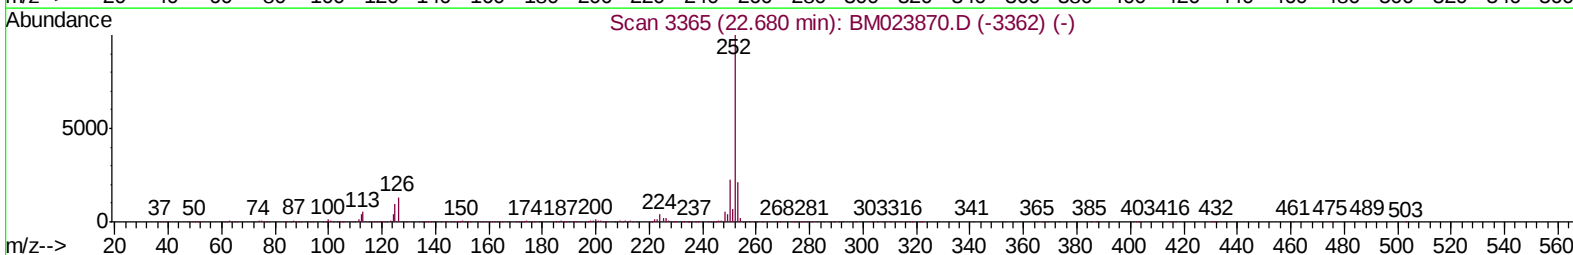
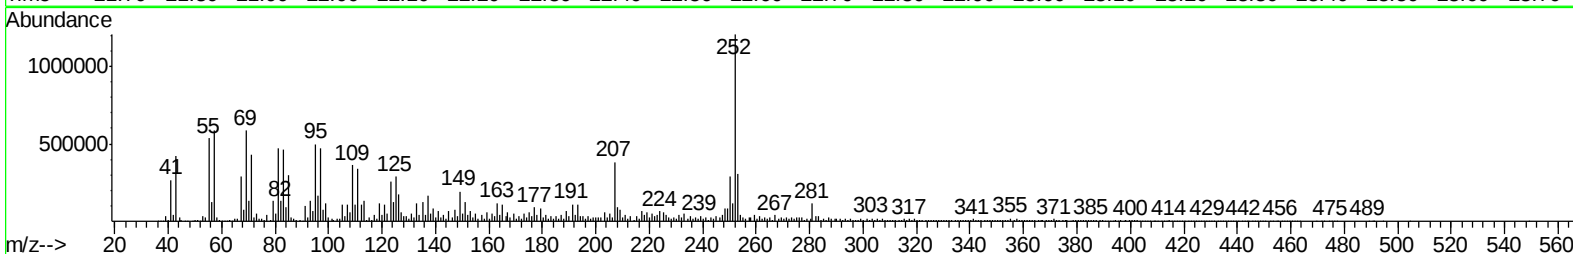


Data File : BM023873.D
Acq On : 23 Nov 2019 00:58
Operator : JU
Sample : K5854-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 25 00:46:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 23 05:21:37 2019
Response via : Initial Calibration

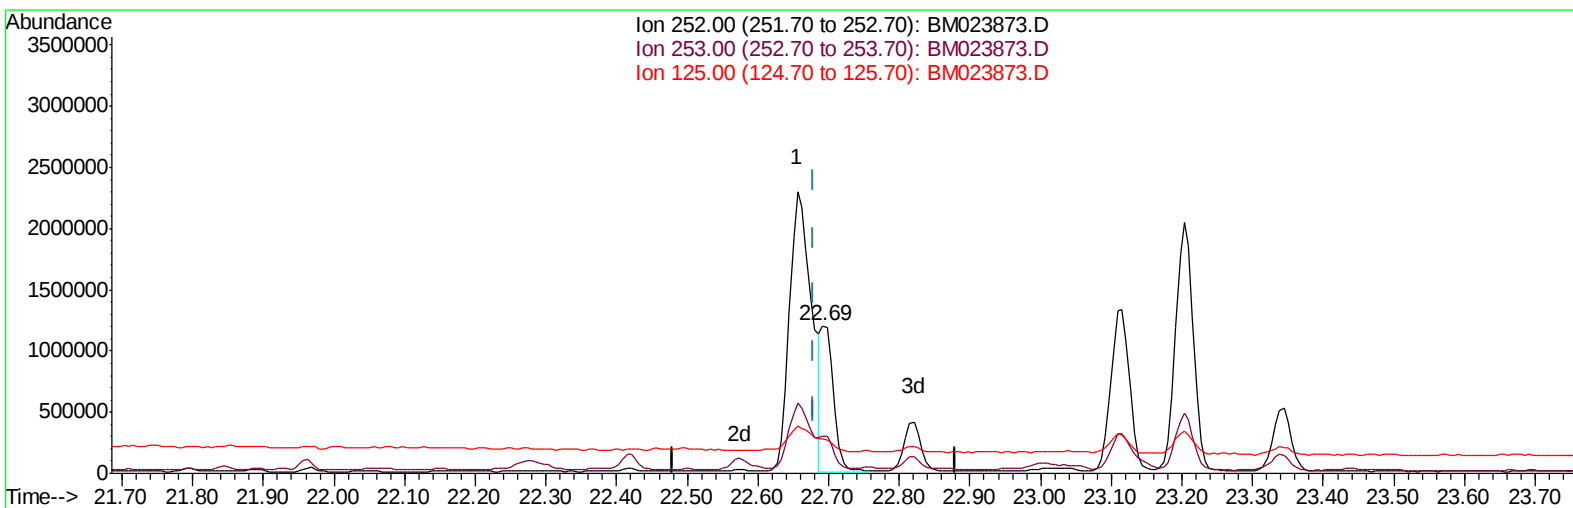

TIC: BM023873.D

(89) Benzo(k)fluoranthene

22.691min (+0.012) 9.15ng/ul m

response 1444175

Ion	Exp%	Act%
252.00	100	100
253.00	21.50	25.25
125.00	7.40	23.76#
0.00	0.00	0.00