

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112219\
 Data File : BM023864.D
 Acq On : 22 Nov 2019 18:22
 Operator : JU
 Sample : K5784-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNA8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	26	28	41	rVB	61097	123125	2.01%	0.177%
2	3.675	130	134	143	rVB	53264	87065	1.42%	0.125%
3	4.669	299	303	306	rBV	31474	46441	0.76%	0.067%
4	5.551	450	453	457	rBV6	3990	6398	0.10%	0.009%
5	6.698	642	648	662	rBV	915151	1634595	26.64%	2.356%
6	6.857	669	675	694	rVB	729254	1199229	19.54%	1.728%
7	7.045	700	707	718	rBV	1011681	1647017	26.84%	2.374%
8	7.145	723	724	730	rVB6	8777	11109	0.18%	0.016%
9	7.510	779	786	796	rBV	1213833	1907993	31.09%	2.750%
10	8.228	901	908	920	rBV	1010273	1692350	27.58%	2.439%
11	8.663	973	982	994	rBV	864786	1475748	24.05%	2.127%
12	9.028	1041	1044	1047	rVB4	5032	6535	0.11%	0.009%
13	9.063	1047	1050	1053	rBV5	4607	7272	0.12%	0.010%
14	9.104	1053	1057	1064	rVB3	24647	45251	0.74%	0.065%
15	9.381	1097	1104	1116	rBV	718443	1227931	20.01%	1.770%
16	9.922	1188	1196	1209	rBV	1112805	1998379	32.56%	2.880%
17	10.286	1250	1258	1266	rBV	1615555	2750304	44.82%	3.964%
18	10.434	1275	1283	1298	rBV	795465	1582507	25.79%	2.281%
19	11.886	1526	1530	1537	rVB	20602	35678	0.58%	0.051%
20	13.016	1717	1722	1726	rVB6	6719	11052	0.18%	0.016%
21	13.504	1800	1805	1810	rVB8	10567	18899	0.31%	0.027%
22	13.586	1812	1819	1824	rVV	2022225	2860527	46.61%	4.122%
23	13.633	1824	1827	1835	rVB	305770	443371	7.22%	0.639%
24	13.857	1858	1865	1880	rBV	2601589	3796091	61.86%	5.471%
25	14.104	1901	1907	1912	rBV9	6121	14967	0.24%	0.022%
26	14.169	1912	1918	1932	rVV	2578876	3805752	62.01%	5.485%
27	14.410	1953	1959	1978	rBV	455221	1085117	17.68%	1.564%
28	14.610	1985	1993	2005	rVB2	147638	259349	4.23%	0.374%
29	14.998	2055	2059	2061	rBV3	10283	16391	0.27%	0.024%
30	15.057	2066	2069	2074	rVB4	14922	20029	0.33%	0.029%
31	15.168	2082	2088	2101	rBV	3306211	4678841	76.24%	6.743%
32	15.310	2106	2112	2121	rVV	616886	889670	14.50%	1.282%
33	15.410	2125	2129	2134	rVB	39667	55069	0.90%	0.079%
34	15.921	2213	2216	2218	rVB4	6537	7216	0.12%	0.010%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112219\
 Data File : BM023864.D
 Acq On : 22 Nov 2019 18:22
 Operator : JU
 Sample : K5784-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNA8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Title : SVOA CALIBRATION

35	15.957	2218	2222	2229	rVB9	17551	27603	0.45%	0.040%
36	16.051	2235	2238	2240	rVB4	5692	6789	0.11%	0.010%
37	16.086	2240	2244	2249	rBV8	7222	14137	0.23%	0.020%
38	16.174	2256	2259	2265	rVB2	18800	26545	0.43%	0.038%
39	16.327	2281	2285	2289	rBV7	10086	14121	0.23%	0.020%
40	16.480	2306	2311	2318	rBV2	41544	63498	1.03%	0.092%
41	16.710	2346	2350	2354	rBV4	23585	33741	0.55%	0.049%
42	16.921	2380	2386	2397	rBV	3160834	4536205	73.92%	6.537%
43	17.021	2397	2403	2415	rVV2	3584279	5003173	81.53%	7.210%
44	17.133	2421	2422	2427	rVB5	18740	22339	0.36%	0.032%
45	17.292	2445	2449	2450	rBV4	11044	10177	0.17%	0.015%
46	17.310	2450	2452	2455	rVV3	6166	8302	0.14%	0.012%
47	17.845	2538	2543	2552	rBV2	167857	318011	5.18%	0.458%
48	18.151	2589	2595	2602	rBV6	36373	91096	1.48%	0.131%
49	18.962	2730	2733	2736	rBV	41349	55063	0.90%	0.079%
50	19.139	2760	2763	2770	rBV9	40486	85412	1.39%	0.123%
51	19.209	2773	2775	2780	rVB2	46178	61598	1.00%	0.089%
52	19.327	2789	2795	2807	rBV	4656847	6136866	100.00%	8.844%
53	20.868	3053	3057	3064	rBV2	690404	1014767	16.54%	1.462%
54	21.127	3096	3101	3110	rBV	3973425	5145185	83.84%	7.415%
55	23.144	3439	3444	3450	rBV	3399168	5842739	95.21%	8.420%
56	23.280	3462	3467	3476	rVB	2991632	5424839	88.40%	7.818%


Sum of corrected areas: 69389474

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112219\
Data File : BM023864.D
Acq On : 22 Nov 2019 18:22
Operator : JU
Sample : K5784-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNA8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

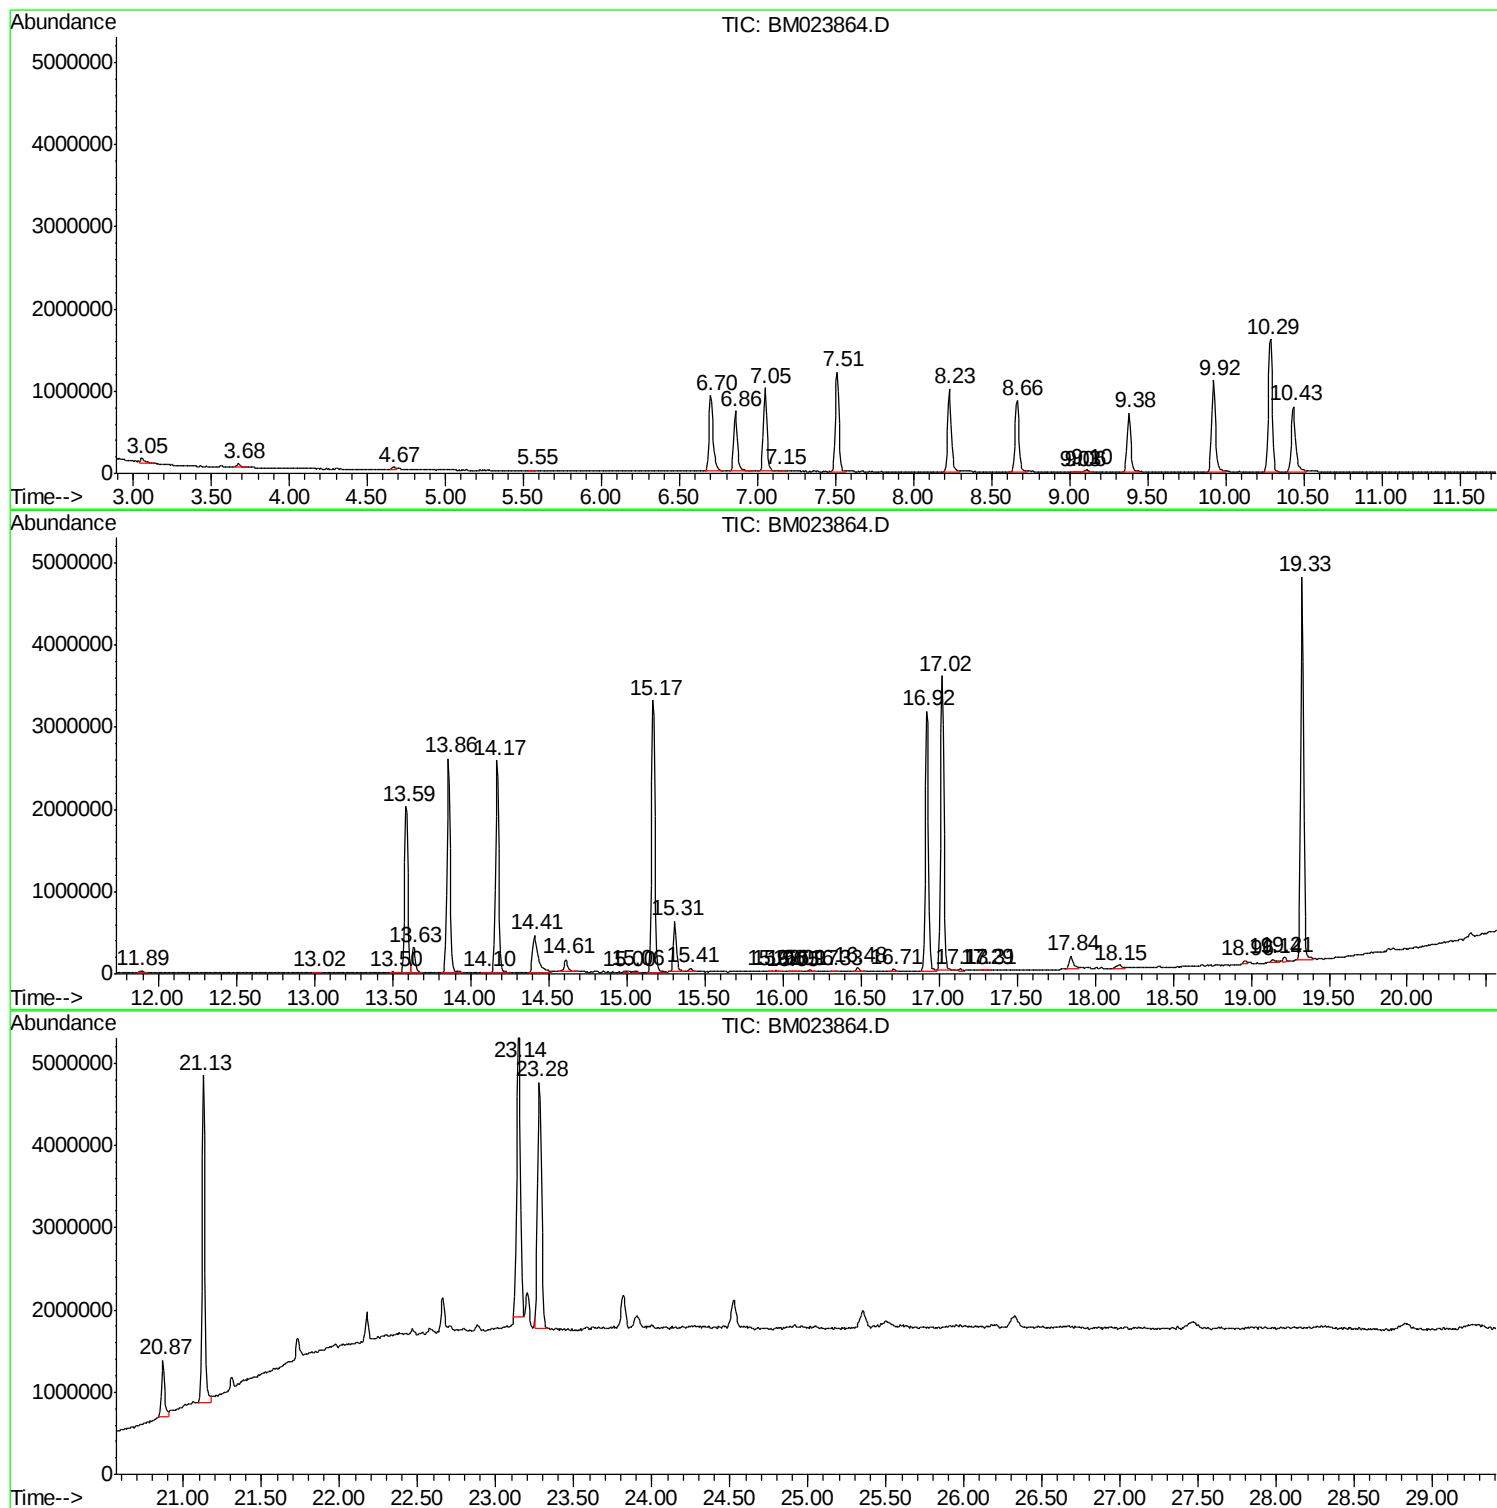

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112219\
Data File : BM023864.D
Acq On : 22 Nov 2019 18:22
Operator : JU
Sample : K5784-01
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
JLNA8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic20.87 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.87	3.94 ng/ul	1014770	Chrysene-d12	21.13
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	5-Octadecene, (E)-	252 C18H36	007206-21-5	96
2	3-Eicosene, (E)-	280 C20H40	074685-33-9	94
3	Heptadecyl heptafluorobutyrate	452 C21H35F7O2	959085-66-6	94
4	n-Nonadecanol-1	284 C19H40O	001454-84-8	93
5	5-Eicosene, (E)-	280 C20H40	074685-30-6	91

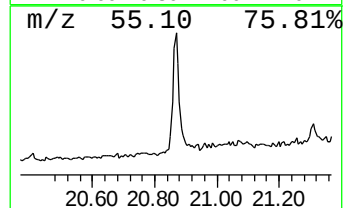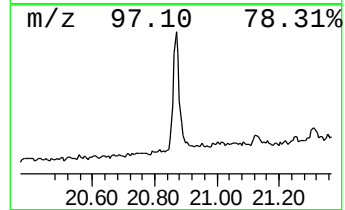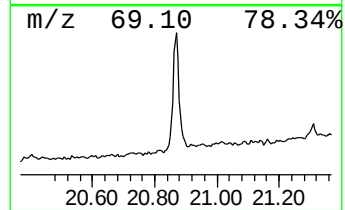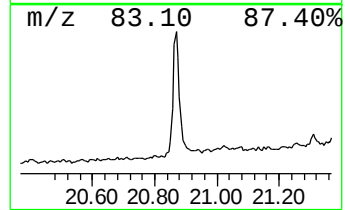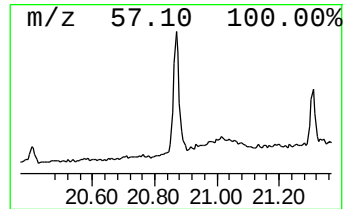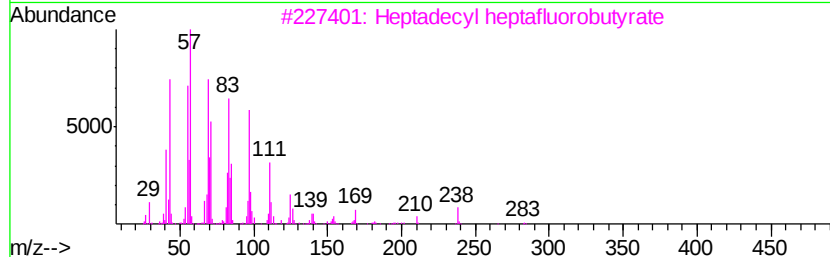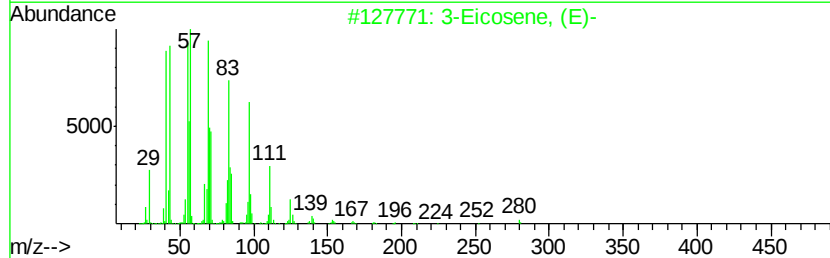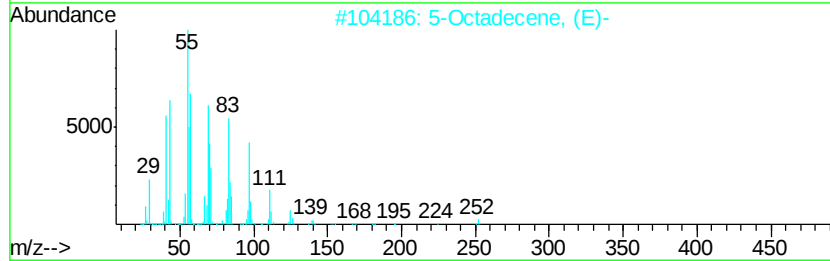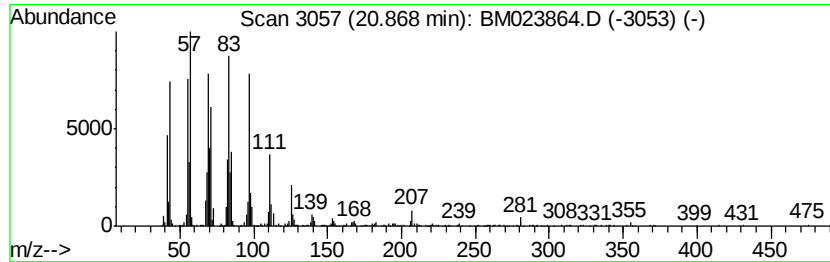

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM112219\
Data File : BM023864.D
Acq On : 22 Nov 2019 18:22
Operator : JU
Sample : K5784-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNA8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Cyc...	20.87	3.9	ng/ul	1014770	5	21.13	5145190	20.0