

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
 Data File : BM042954.D
 Acq On : 22 Nov 2023 16:17
 Operator : MA/JU
 Sample : PB157008BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK008

Quant Time: Nov 23 00:11:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 22 10:35:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	807	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.618	136	1921	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.465	164	1028	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.314	188	219447	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.41
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.77
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	7141	5.631	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.251	152	811	0.335	ng/ul	0.02
18) Fluoranthene-d10	19.253	212	1793	0.000	ng/ul	0.00
Target Compounds						
12) Fluorene	15.455	166	534	0.104	ng/ul#	Qvalue 21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
Data File : BM042954.D
Acq On : 22 Nov 2023 16:17
Operator : MA/JU
Sample : PB157008BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK008


Quant Time: Nov 23 00:11:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 22 10:35:26 2023
Response via : Initial Calibration

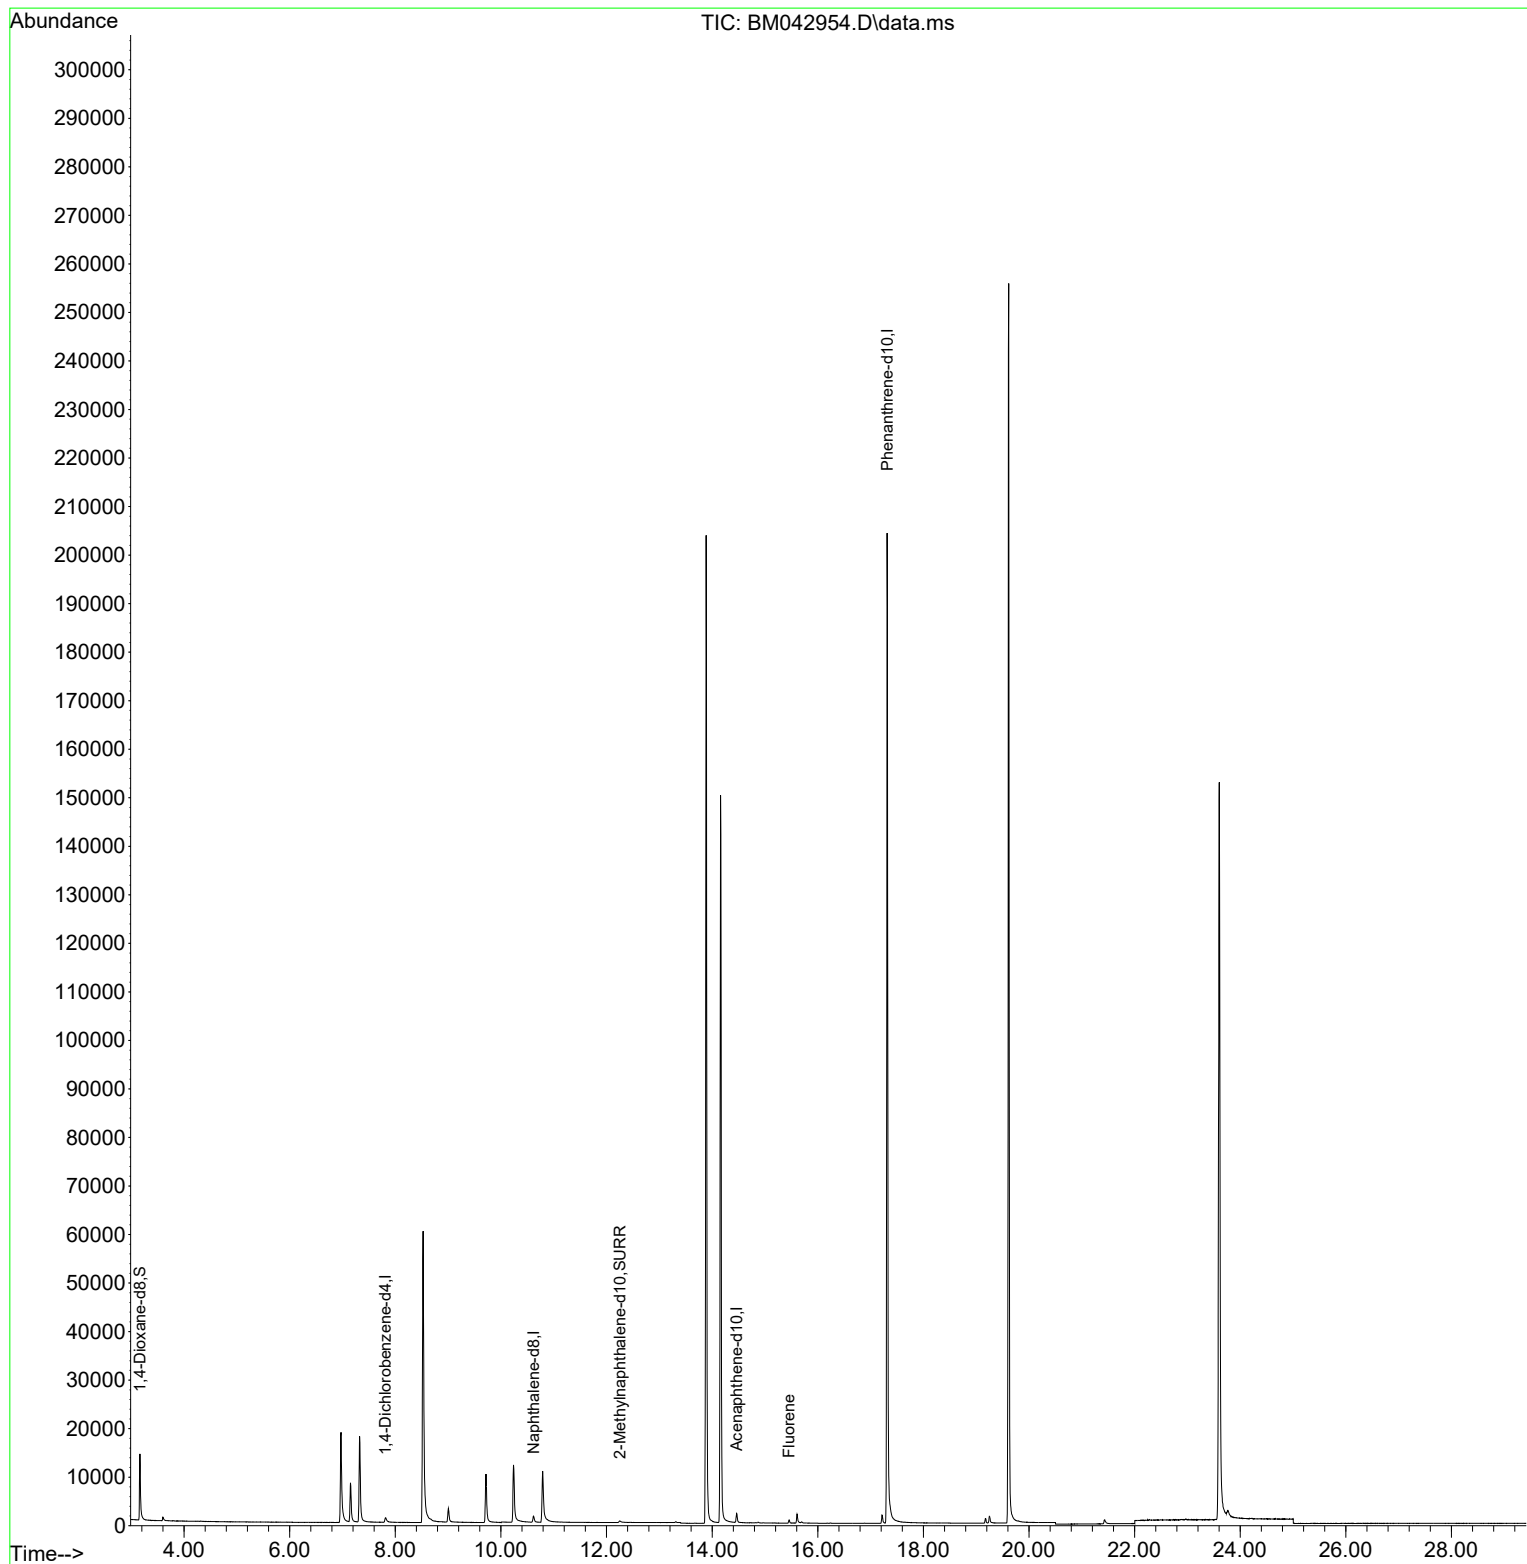

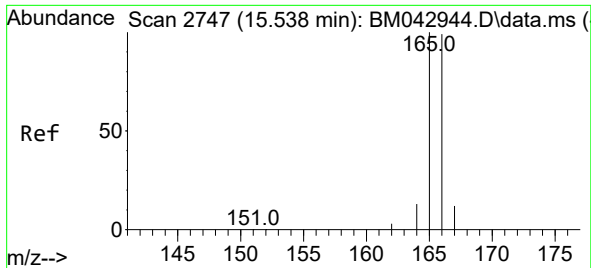

#12
 Fluorene
 Concen: 0.104 ng/ul
 RT: 15.455 min Scan# 21
 Delta R.T. -0.073 min
 Lab File: BM042954.D
 Acq: 22 Nov 2023 16:17

Instrument :
 BNA_M
 ClientSampleId :
 SBLK008

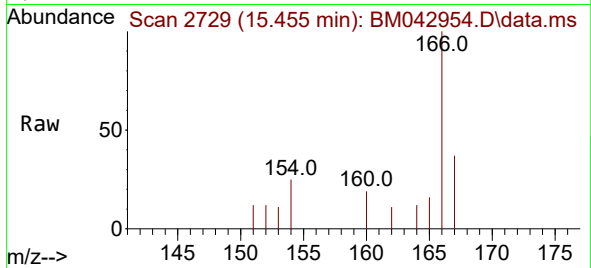

Tgt Ion:166 Resp: 534
 Ion Ratio Lower Upper
 166 100
 165 16.3 84.3 126.5#
 167 36.8 15.0 22.6#

