

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
 Data File : BM042956.D
 Acq On : 22 Nov 2023 17:30
 Operator : MA/JU
 Sample : 05268-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD3

Quant Time: Nov 23 00:11:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 22 10:35:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	787	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.616	136	1937	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.464	164	1061	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.317	188	238194	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.41
23) Perylene-d12	23.768	264	3843	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	4708	3.807	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.239	152	765	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.252	212	1965	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.202	88	57	0.041	ng/ul#	80
26) Benzo(a)pyrene	23.604	252	1203	0.076	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
Data File : BM042956.D
Acq On : 22 Nov 2023 17:30
Operator : MA/JU
Sample : 05268-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD3

Quant Time: Nov 23 00:11:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 22 10:35:26 2023
Response via : Initial Calibration

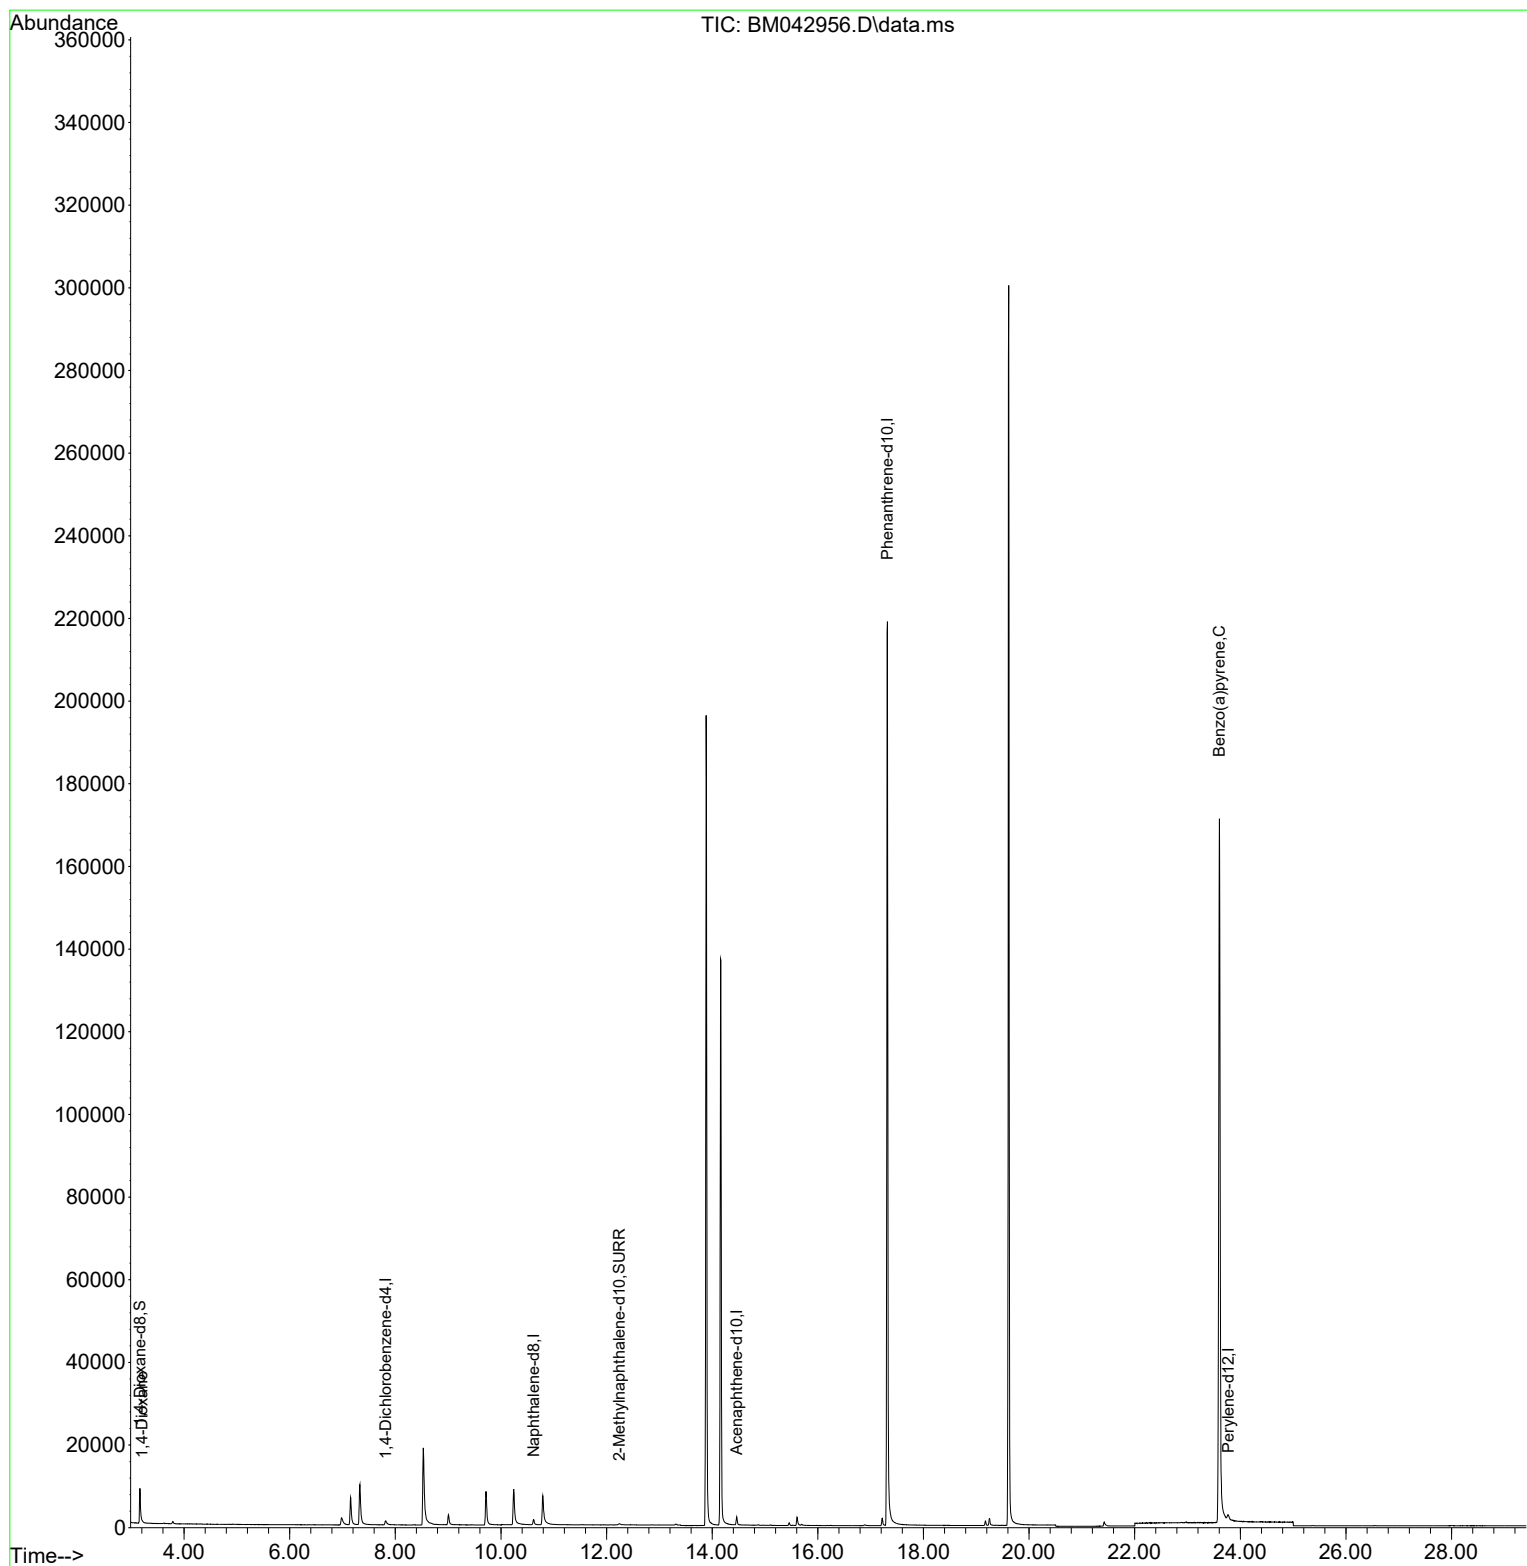

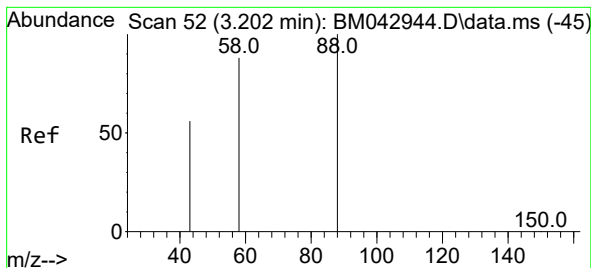

#2

1,4-Dioxane

Concen: 0.041 ng/ul

RT: 3.202 min Scan# 51

Delta R.T. -0.004 min

Lab File: BM042956.D

Acq: 22 Nov 2023 17:30

Instrument :

BNA_M

ClientSampleId :

DCKD3





Tgt Ion: 88 Resp: 57

Ion Ratio Lower Upper

88 100

43 53.2 30.5 45.7#

58 20.2 21.8 32.6#

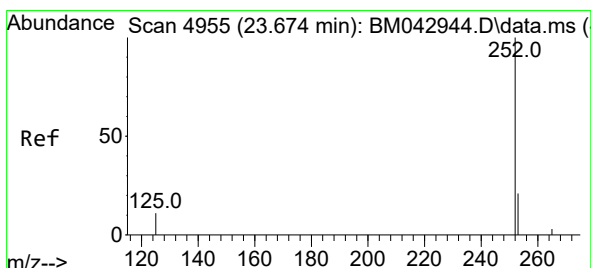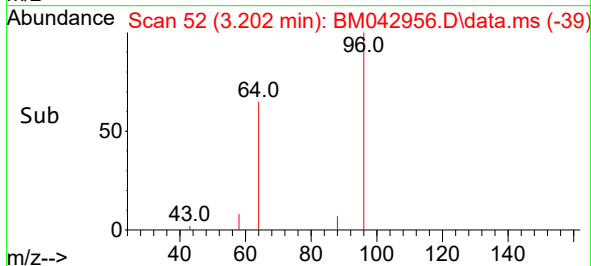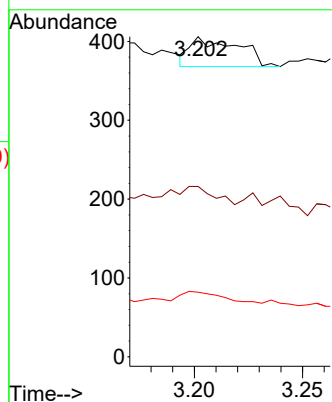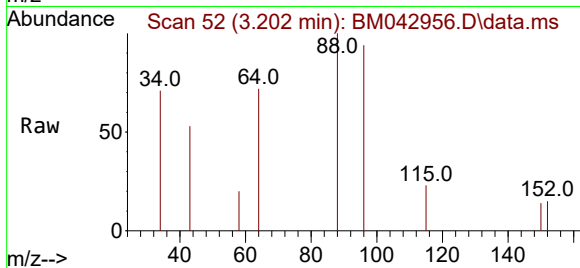

#26

Benzo(a)pyrene

Concen: 0.076 ng/ul

RT: 23.604 min Scan# 4931

Delta R.T. -0.064 min

Lab File: BM042956.D

Acq: 22 Nov 2023 17:30

Tgt Ion: 252 Resp: 1203

Ion Ratio Lower Upper

252 100

253 57.6 35.1 52.7#

125 45.7 21.2 31.8#

