

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
 Data File : BM042960.D
 Acq On : 22 Nov 2023 19:56
 Operator : MA/JU
 Sample : 05268-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD8

Quant Time: Nov 23 00:12:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 22 10:35:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	593	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.616	136	1506	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.464	164	829	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.313	188	216225	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.41
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.77
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	3409	3.658	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.250	152	624	0.329	ng/ul	0.02
18) Fluoranthene-d10	19.252	212	1895	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.176	88	36	0.035	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
Data File : BM042960.D
Acq On : 22 Nov 2023 19:56
Operator : MA/JU
Sample : 05268-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD8

Quant Time: Nov 23 00:12:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 22 10:35:26 2023
Response via : Initial Calibration

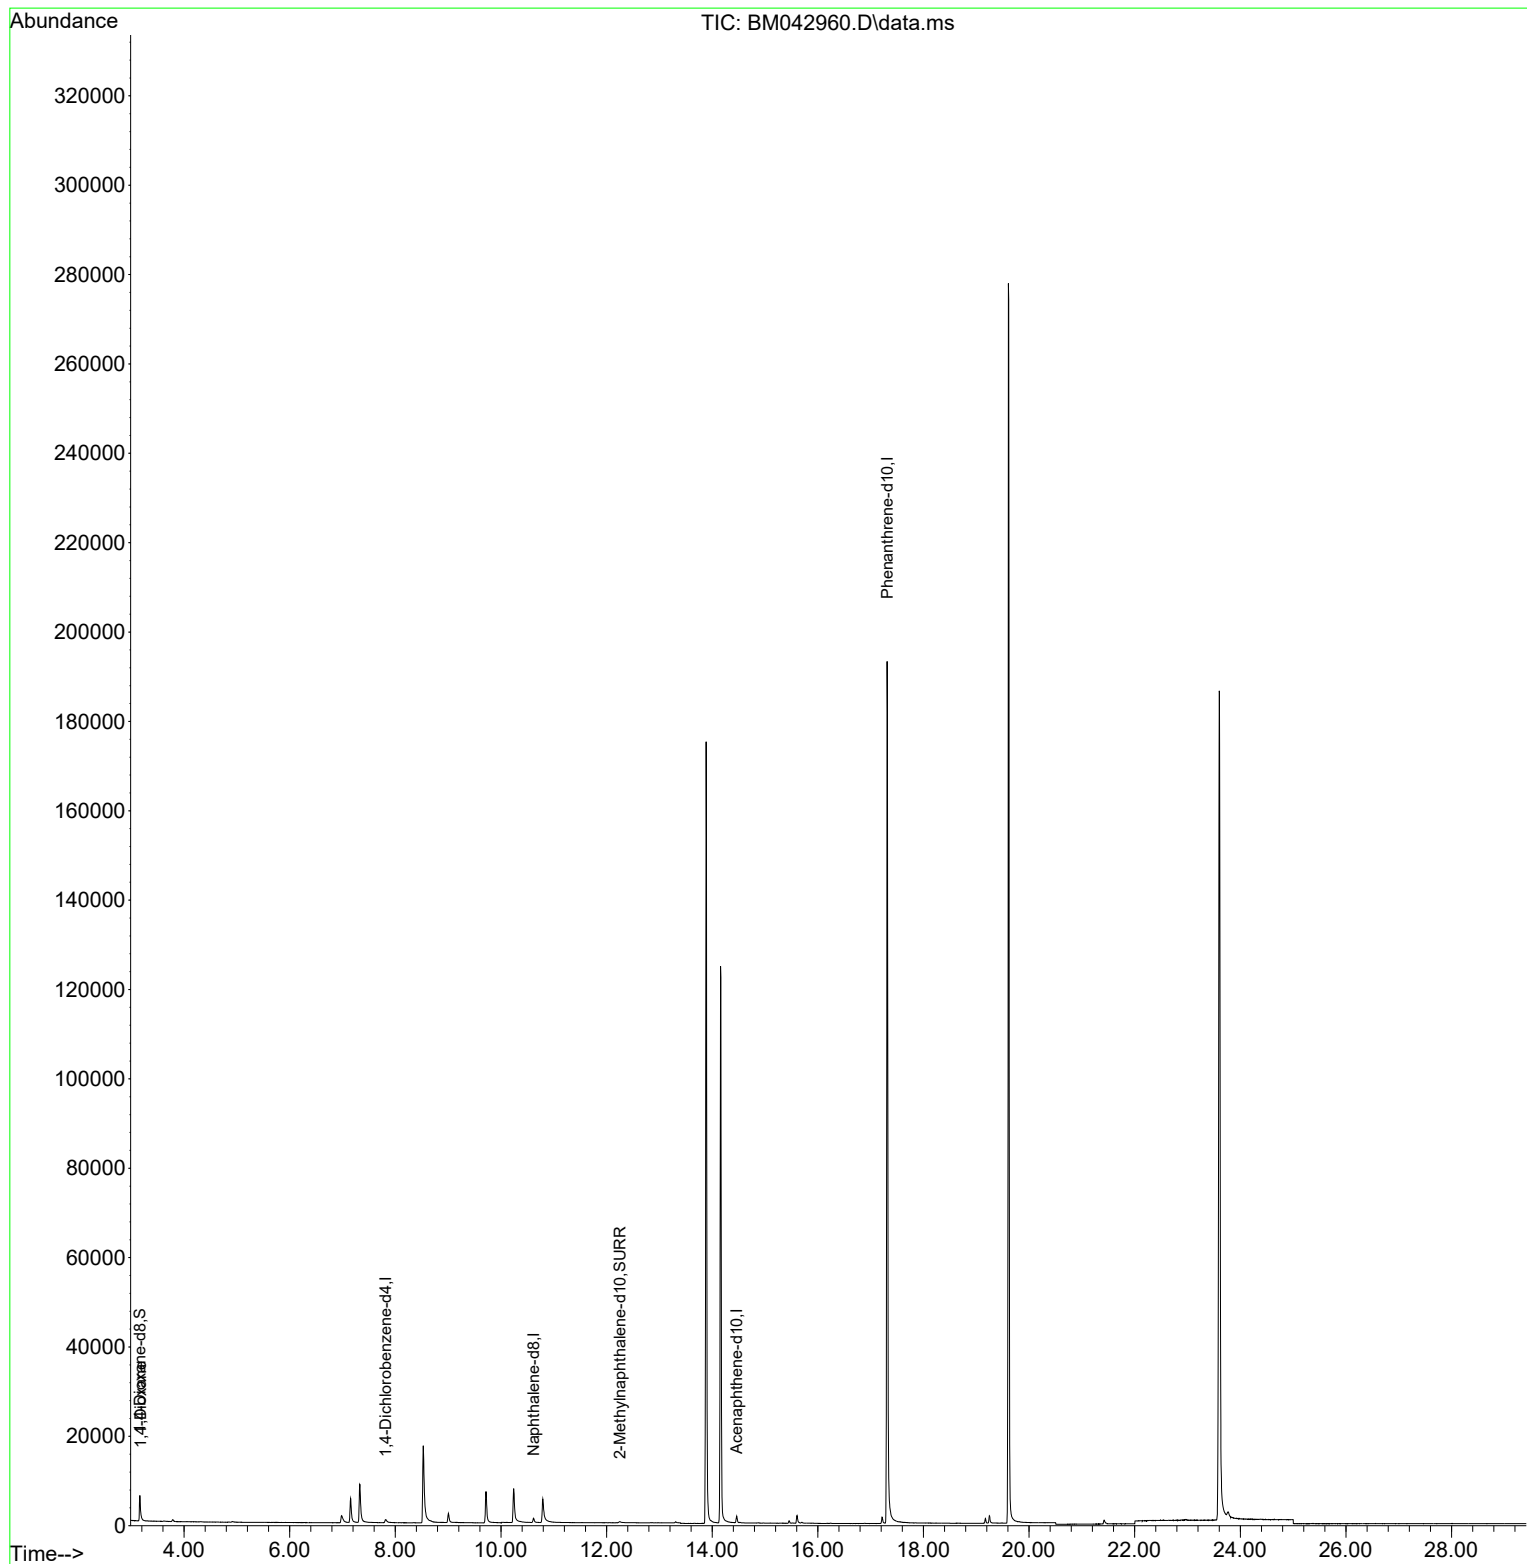

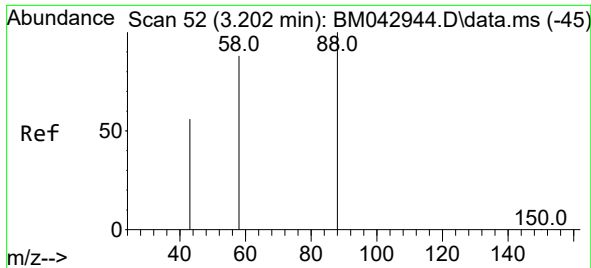

#2

1,4-Dioxane

Concen: 0.035 ng/ul

RT: 3.176 min Scan# 4

Delta R.T. -0.029 min

Lab File: BM042960.D


Acq: 22 Nov 2023 19:56

Instrument :

BNA_M

ClientSampleId :

DCKD8

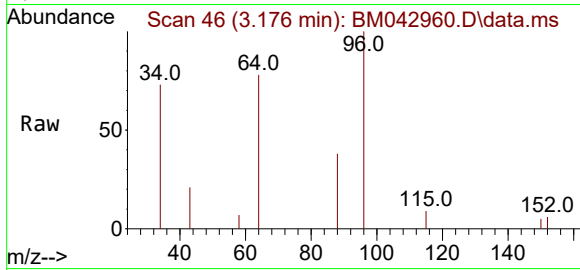

Tgt Ion: 88 Resp: 36

Ion Ratio Lower Upper

88 100

43 54.4 30.5 45.7#

58 18.0 21.8 32.6#

