

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
 Data File : BM042964.D
 Acq On : 22 Nov 2023 22:22
 Operator : MA/JU
 Sample : 05268-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD1

Quant Time: Nov 23 00:12:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 22 10:35:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	783	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.616	136	1874	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.464	164	1063	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.313	188	269065	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.41
23) Perylene-d12	23.762	264	4024	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	4054	3.295	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	873	0.370	ng/ul	0.00
18) Fluoranthene-d10	19.247	212	2418	0.000	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.202	88	29	0.021	ng/ul#	79
12) Fluorene	15.454	166	608	0.114	ng/ul#	21
26) Benzo(a)pyrene	23.601	252	1484	0.089	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
Data File : BM042964.D
Acq On : 22 Nov 2023 22:22
Operator : MA/JU
Sample : 05268-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD1

Quant Time: Nov 23 00:12:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 22 10:35:26 2023
Response via : Initial Calibration




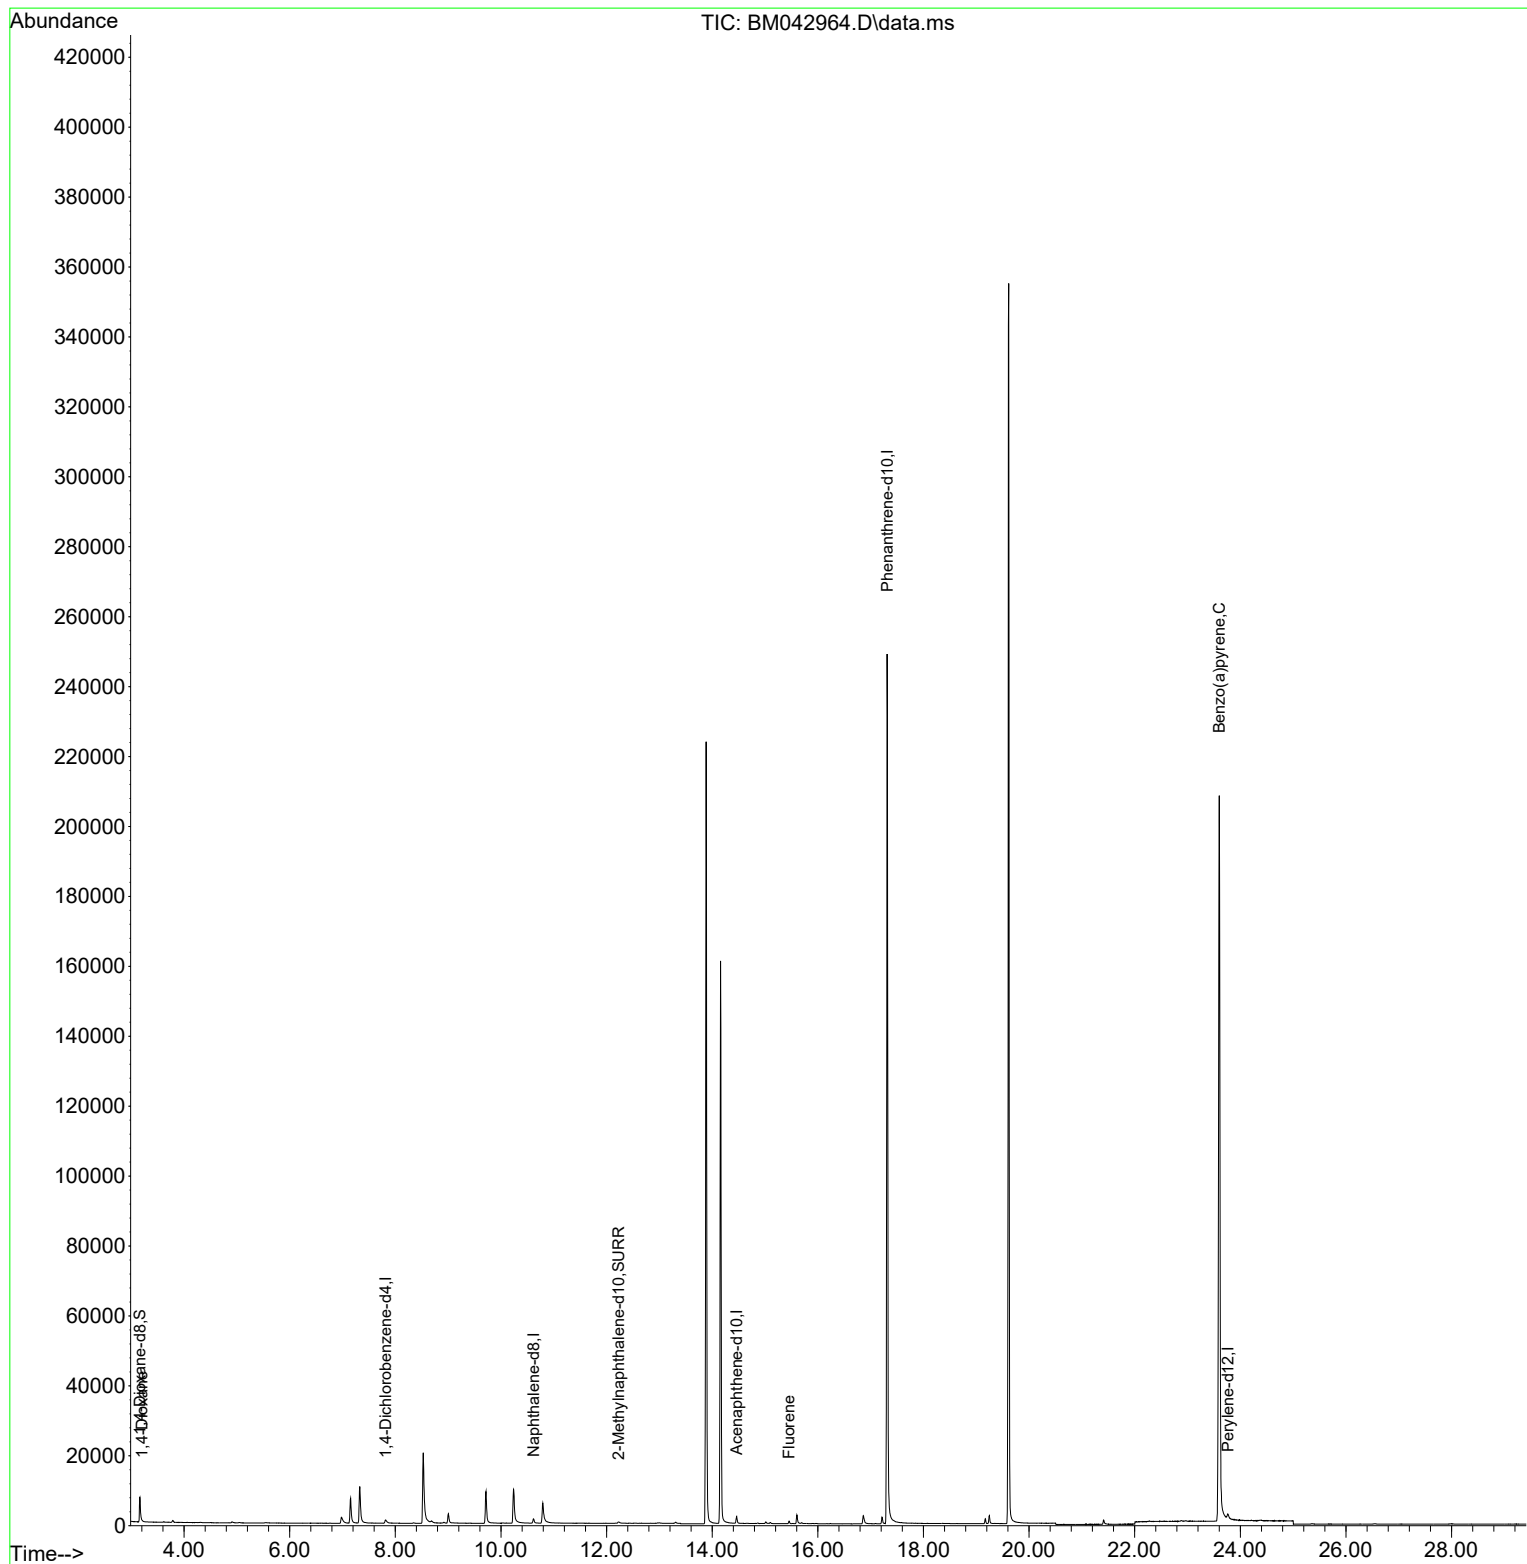


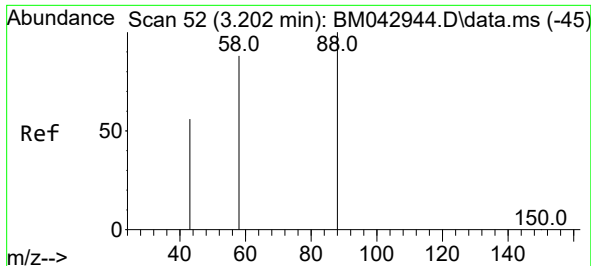

#2
1,4-Dioxane
Concen: 0.021 ng/ul
RT: 3.202 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM042964.D
Acq: 22 Nov 2023 22:22




Instrument :
BNA_M
ClientSampleId :
DCKD1


Tgt Ion: 88 Resp: 29
Ion Ratio Lower Upper
88 100
43 54.8 30.5 45.7#
58 21.3 21.8 32.6#

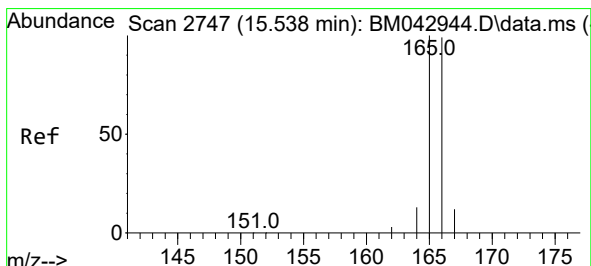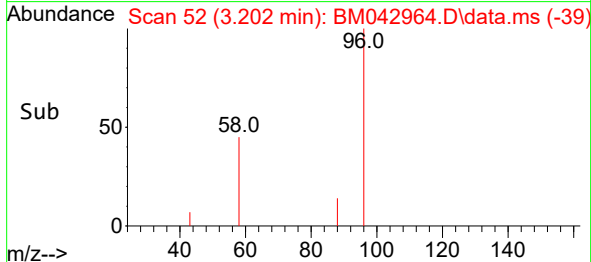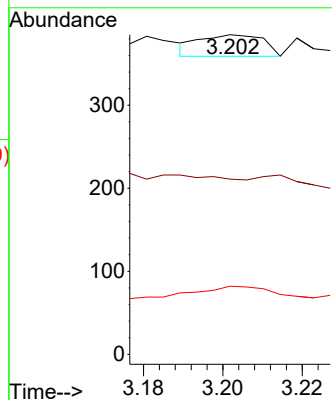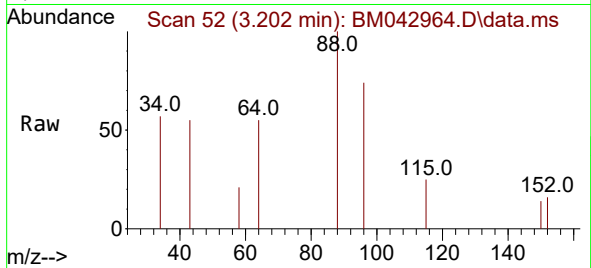

#12
Fluorene
Concen: 0.114 ng/ul
RT: 15.454 min Scan# 2729
Delta R.T. -0.074 min
Lab File: BM042964.D
Acq: 22 Nov 2023 22:22


Tgt Ion: 166 Resp: 608
Ion Ratio Lower Upper
166 100
165 16.7 84.3 126.5#
167 37.7 15.0 22.6#

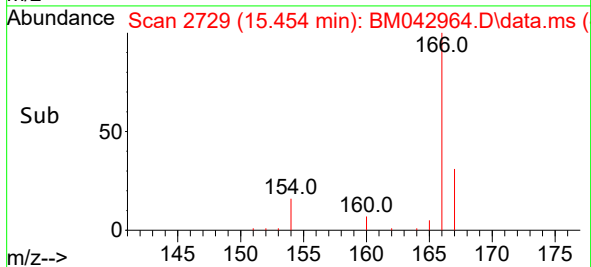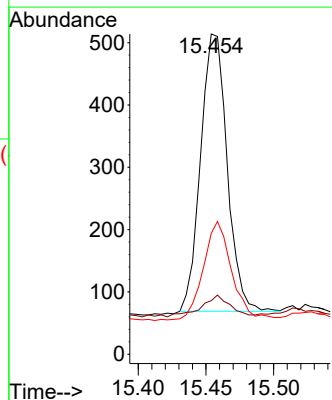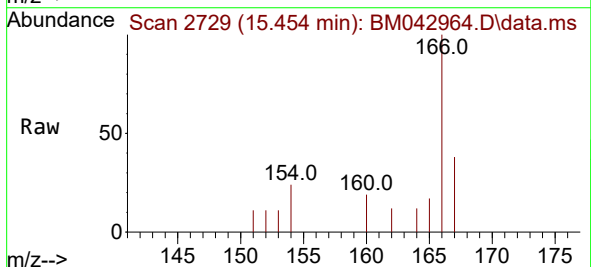

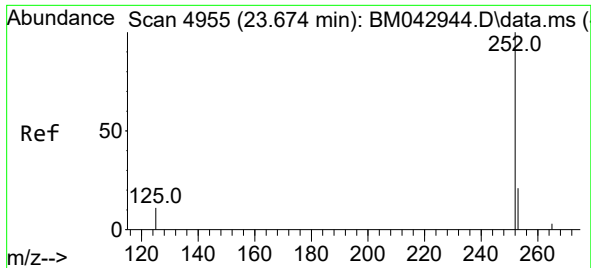

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.601 min Scan# 4930
Delta R.T. -0.067 min
Lab File: BM042964.D
Acq: 22 Nov 2023 22:22

Instrument :
BNA_M
ClientSampleId :
DCKD1

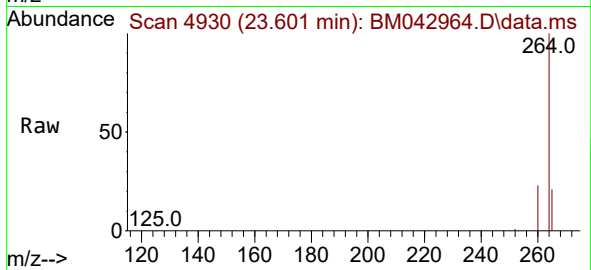

Tgt Ion:252 Resp: 1484
Ion Ratio Lower Upper
252 100
253 56.4 35.1 52.7#
125 44.3 21.2 31.8#

