




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
 Data File : BM042946.D
 Acq On : 22 Nov 2023 11:07
 Operator : MA/JU
 Sample : 05268-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKF9

Manual IntegrationsAPPROVED

Quant Time: Nov 23 04:22:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 22 10:35:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

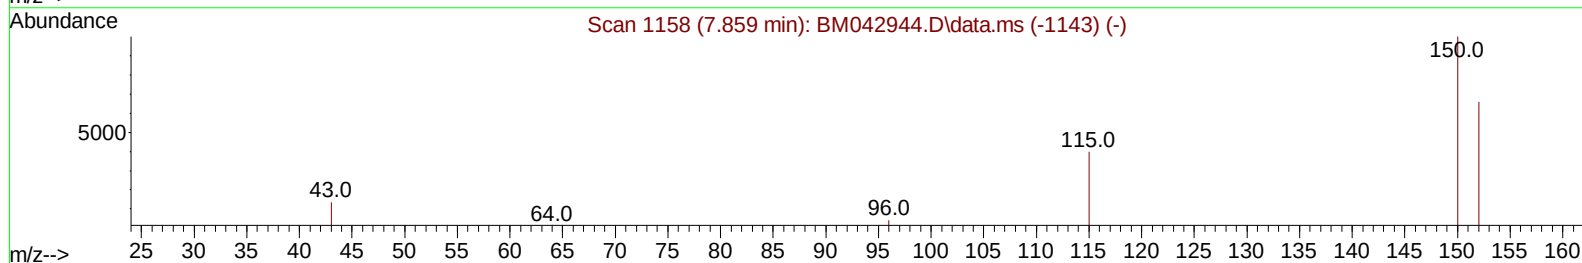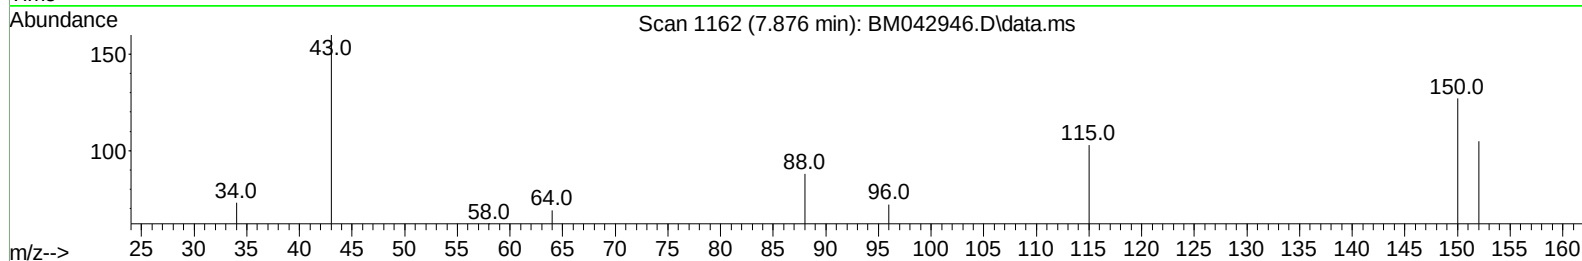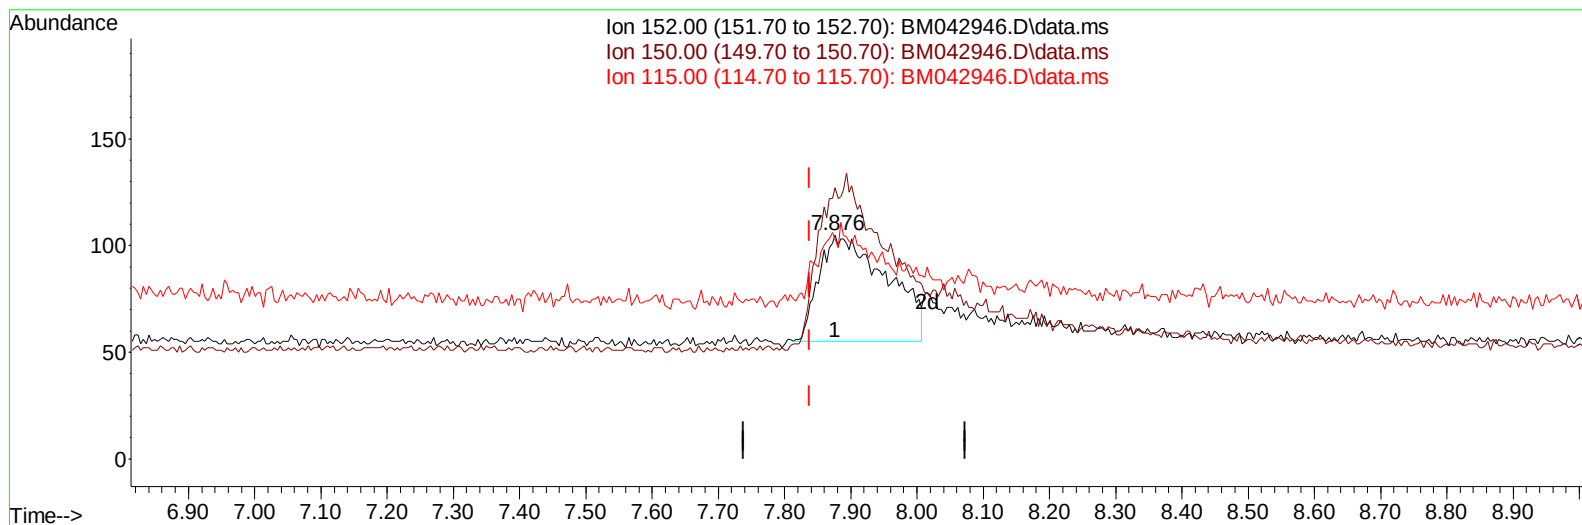

TIC: BM042946.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.876min (+ 0.038) 0.40 ng/u1

response 354

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	142.70	120.95
115.00	84.90	98.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
Data File : BM042946.D
Acq On : 22 Nov 2023 11:07
Operator : MA/JU
Sample : 05268-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKF9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 11:36:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 22 10:35:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

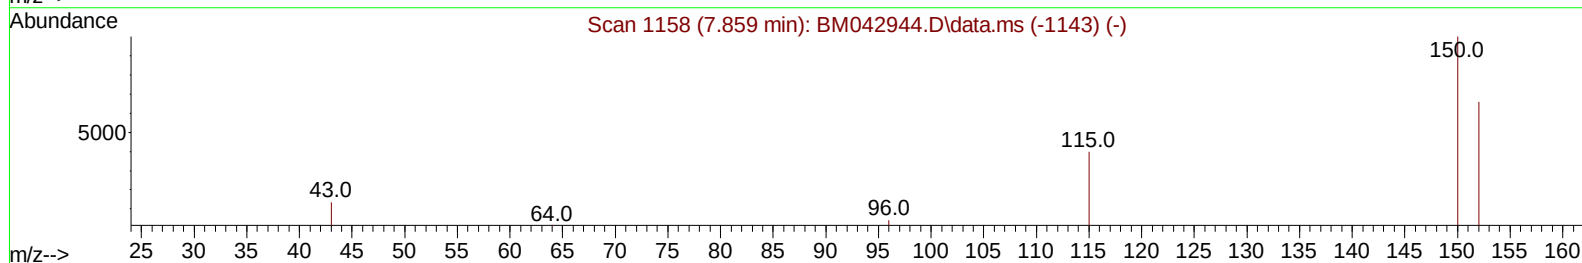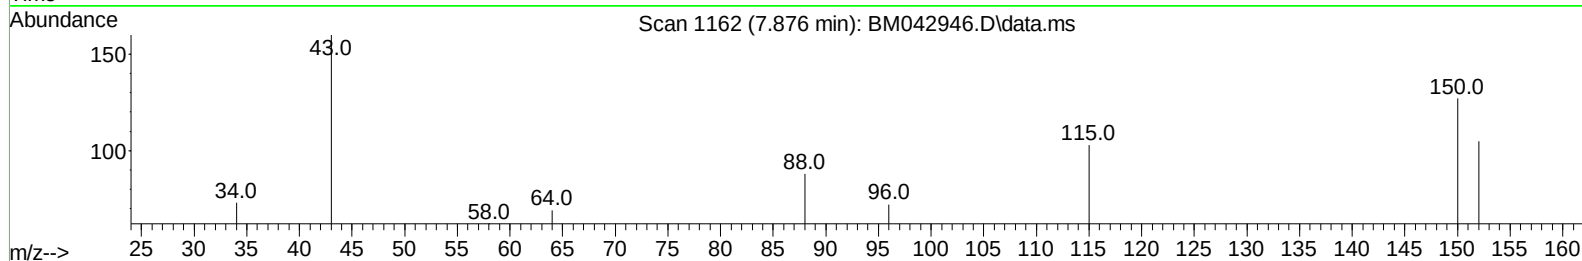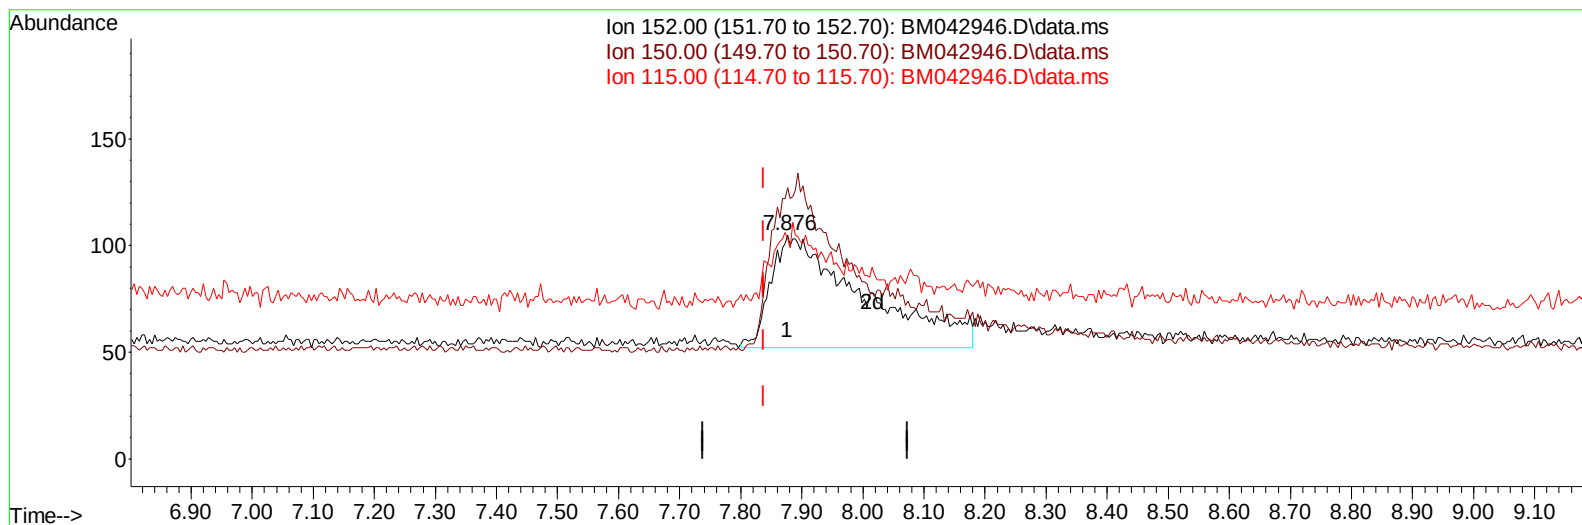

TIC: BM042946.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.876min (+ 0.038) 0.40 ng/ul m

response 552

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	142.70	120.95
115.00	84.90	98.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
 Data File : BM042946.D
 Acq On : 22 Nov 2023 11:07
 Operator : MA/JU
 Sample : 05268-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKF9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 11:36:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 22 10:35:26 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.876	152		552m	0.400	ng/ul	0.04
4) Naphthalene-d8	10.667	136		1226	0.400	ng/ul	# 0.03
9) Acenaphthene-d10	14.474	164		679	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.226	188		1565	0.400	ng/ul	0.00
17) Chrysene-d12	21.426	240		1014	0.400	ng/ul	0.01
23) Perylene-d12	23.785	264		1447	0.400	ng/ul	0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.181	96		619	0.714	ng/ul	0.01
6) 2-Methylnaphthalene-d10	12.262	152		578	0.374	ng/ul	0.03
18) Fluoranthene-d10	19.253	212		1648	0.499	ng/ul	0.00
Target Compounds							Qvalue
14) Pentachlorophenol	16.858	266		6965	8.004	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
Data File : BM042946.D
Acq On : 22 Nov 2023 11:07
Operator : MA/JU
Sample : 05268-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKF9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 11:36:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 22 10:35:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

