

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
 Data File : BM042964.D
 Acq On : 22 Nov 2023 22:22
 Operator : MA/JU
 Sample : 05268-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/25/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 23 00:12:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 22 10:35:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	783	0.400	ng/u1	-0.02
4) Naphthalene-d8	10.616	136	1874	0.400	ng/u1	-0.02
9) Acenaphthene-d10	14.464	164	1063	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.216	188	2484m	0.400	ng/u1	-0.01
17) Chrysene-d12	21.412	240	1509m	0.400	ng/u1	0.00
23) Perylene-d12	23.762	264	4024	0.400	ng/u1	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	4054	3.295	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.228	152	873	0.370	ng/u1	0.00
18) Fluoranthene-d10	19.247	212	2418	0.492	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.861	266	2347	1.699	ng/u1	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM112223\
Data File : BM042964.D
Acq On : 22 Nov 2023 22:22
Operator : MA/JU
Sample : 05268-09
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DCKD1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2023
Supervised By :mohammad ahmed 11/25/2023


Quant Time: Nov 23 00:12:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM112123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 22 10:35:26 2023
Response via : Initial Calibration

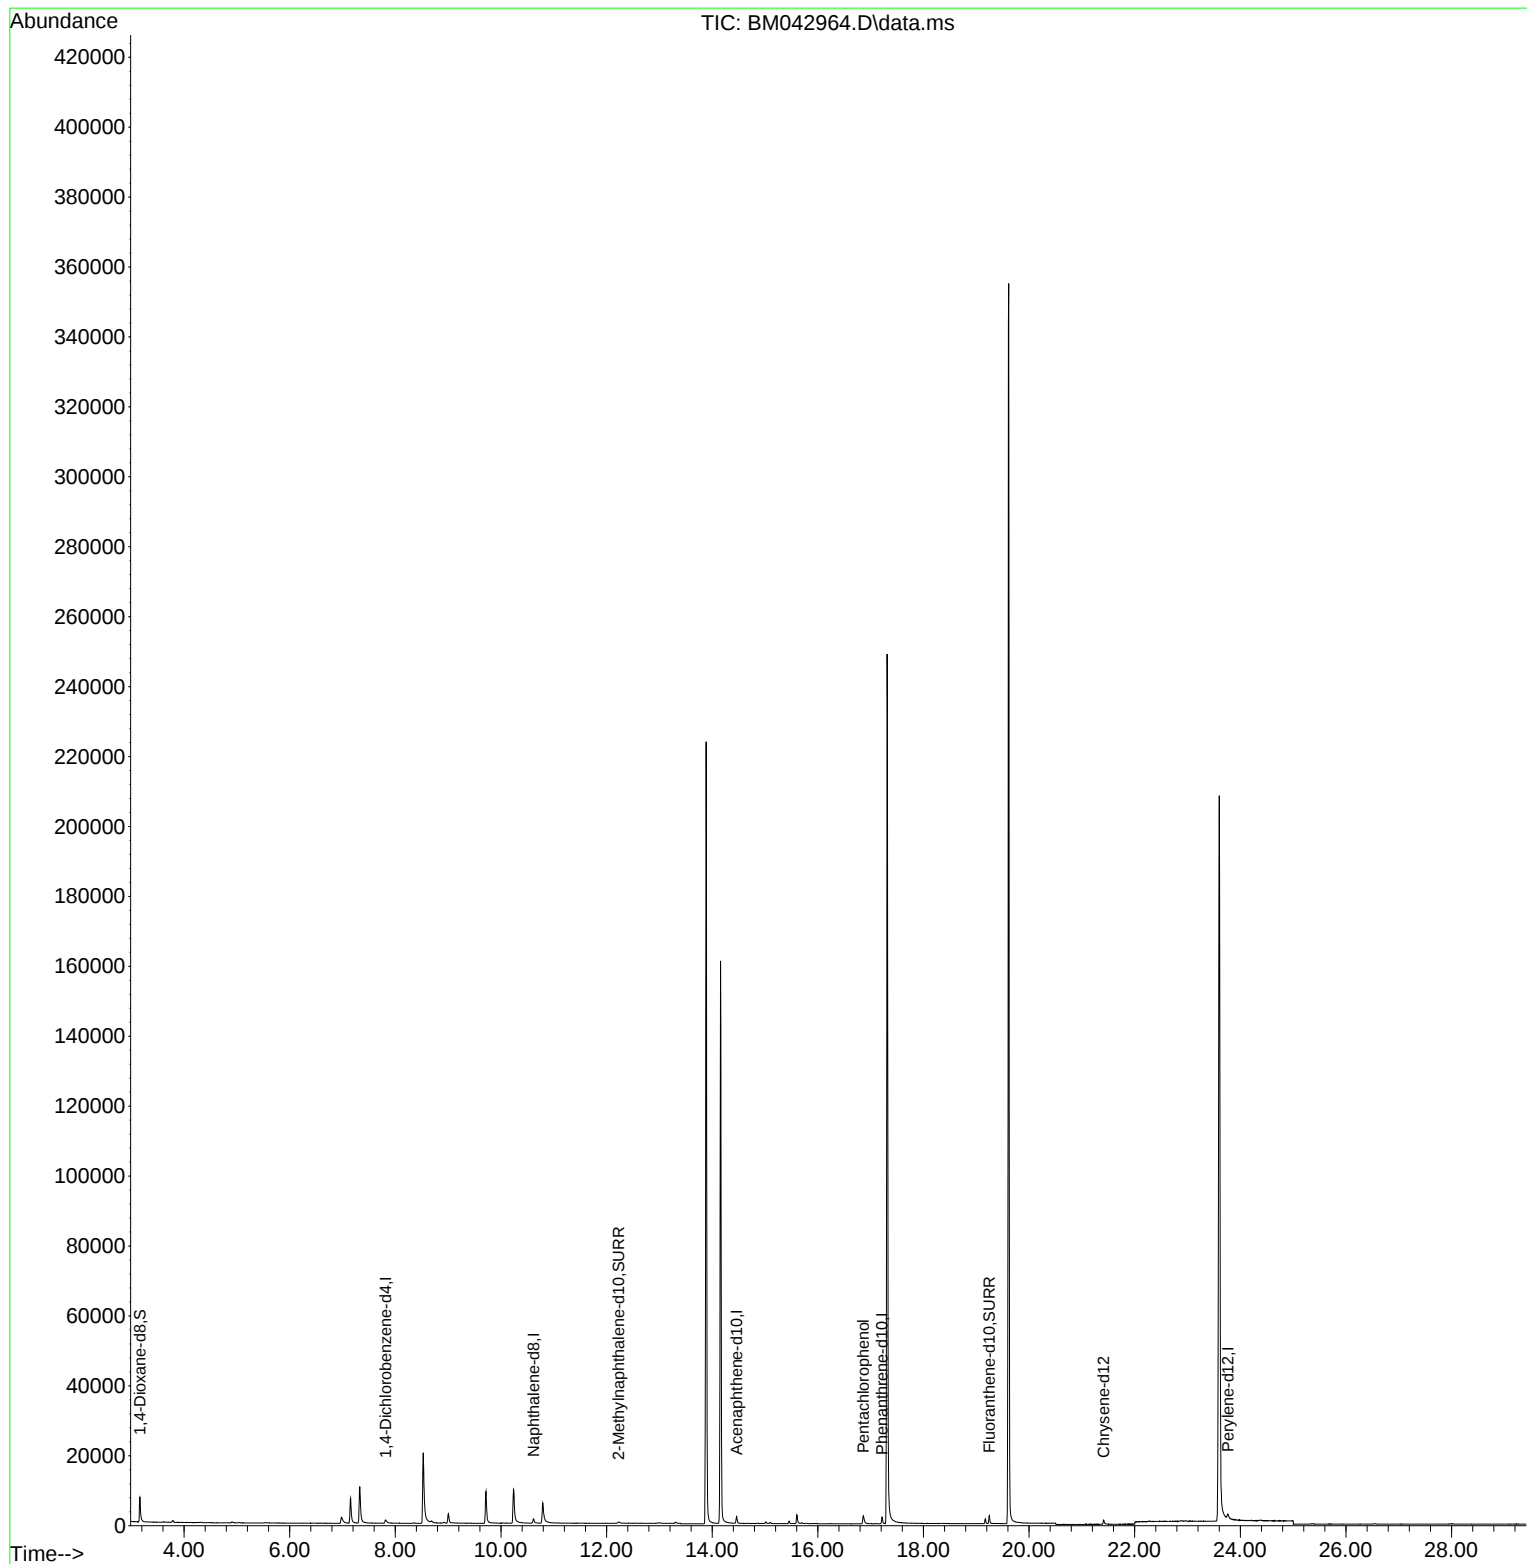

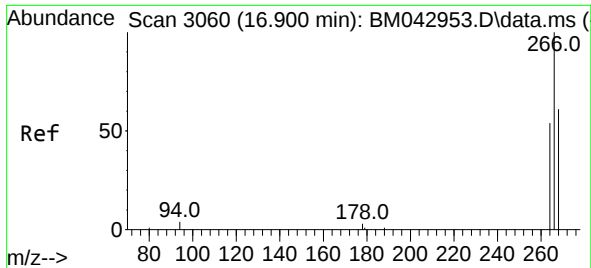

#14
 Pentachlorophenol
 Concen: 1.699 ng/ul
 RT: 16.861 min Scan# 30
 Delta R.T. -0.029 min
 Lab File: BM042964.D
 Acq: 22 Nov 2023 22:22

Instrument :
 BNA_M
 ClientSampleId :
 DCKD1

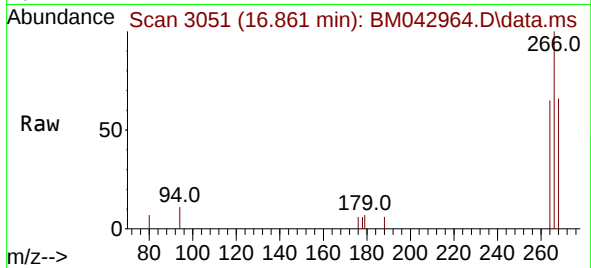

Tgt Ion	Ratio	Lower	Upper
266	100		
264	61.6	52.2	78.2
268	62.8	48.0	72.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/25/2023
 Supervised By :mohammad ahmed 11/25/2023

